

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031224\
 Data File : VW028153.D
 Acq On : 12 Mar 2024 12:41
 Operator : SY/MD
 Sample : P1715-17
 Misc : 4.96g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 13 01:10:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 13 01:09:10 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	417081	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	369415	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	190112	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	94253	18.931	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.720%		
7) Chloroethane-d5	2.905	69	68939	17.875	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.480%		
11) 1,1-Dichloroethene-d2	4.021	65	39880	19.610	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.440%		
21) 2-Butanone-d5	7.075	46	26335	37.080	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.160%		
24) Chloroform-d	7.648	84	162920	18.443	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	73.760%		
26) 1,2-Dichloroethane-d4	8.301	65	79815	19.414	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.640%		
32) Benzene-d6	8.276	84	346144	20.072	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	80.280%		
36) 1,2-Dichloropropane-d6	9.270	67	85815	19.260	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	77.040%		
41) Toluene-d8	10.319	98	324248	19.951	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	79.800%		
43) trans-1,3-Dichloroprop...	10.575	79	37743	19.330	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.320%		
47) 2-Hexanone-d5	10.922	63	24961	39.773	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.540%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	67079	19.075	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	76.280%		
66) 1,2-Dichlorobenzene-d4	13.849	152	111626	19.743	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	78.960%		
Target Compounds			Qvalue			
39) cis-1,3-Dichloropropene	10.032	75	2902	0.380	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031224\
Data File : VW028153.D
Acq On : 12 Mar 2024 12:41
Operator : SY/MD
Sample : P1715-17
Misc : 4.96g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 13 01:10:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 13 01:09:10 2024
Response via : Initial Calibration

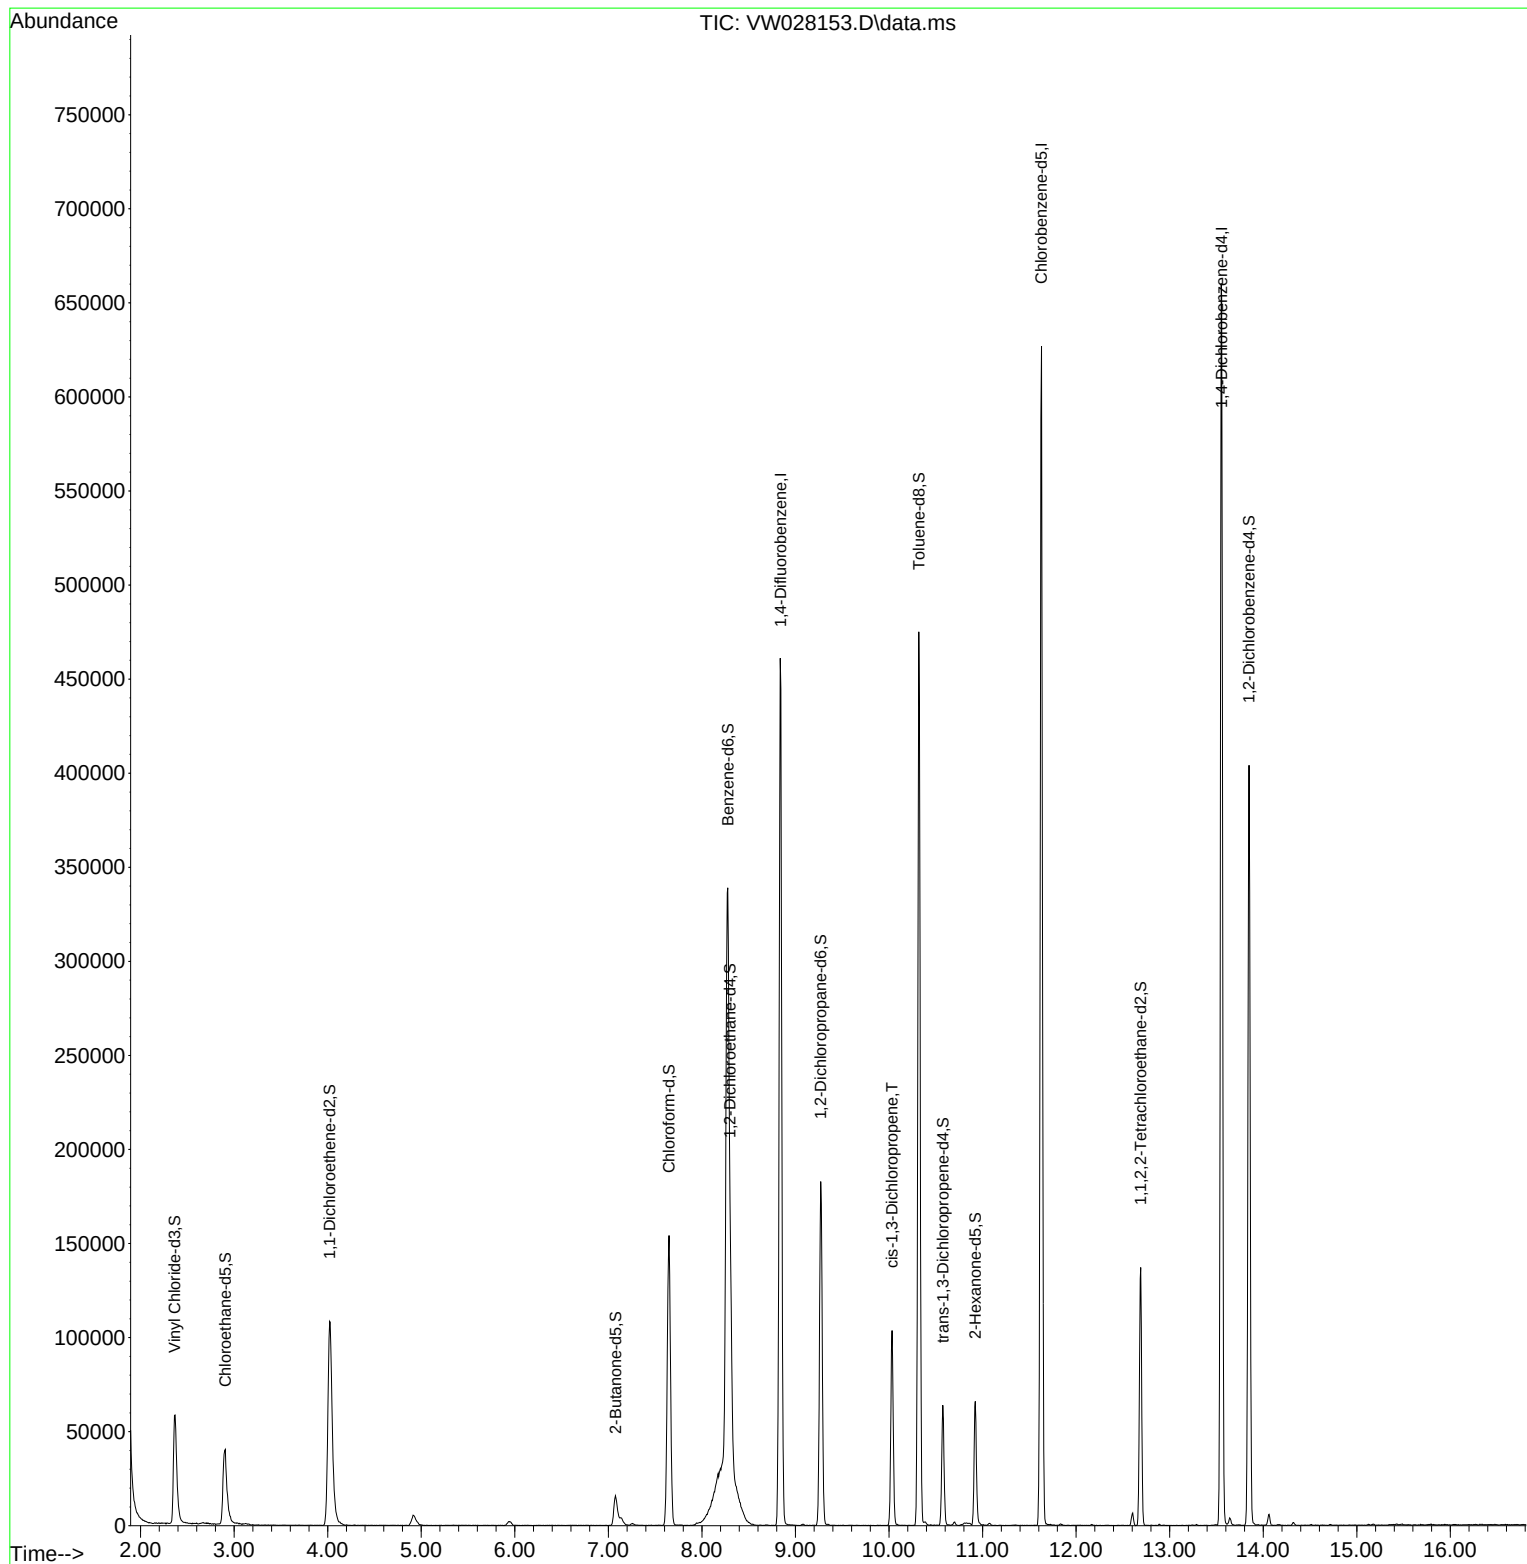

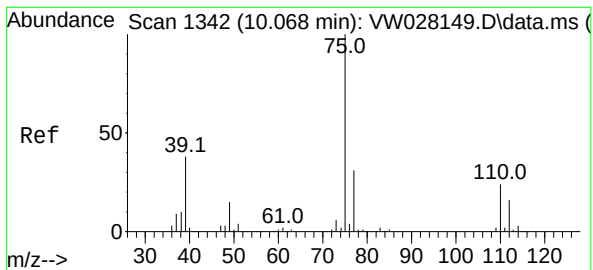

#39

cis-1,3-Dichloropropene

Concen: 0.380 ug/L

RT: 10.032 min Scan# 14

Delta R.T. -0.036 min

Lab File: VW028153.D

Acq: 12 Mar 2024 12:41

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 2902

Ion	Ratio	Lower	Upper
75	100		
77	48.4	21.7	40.3#

