
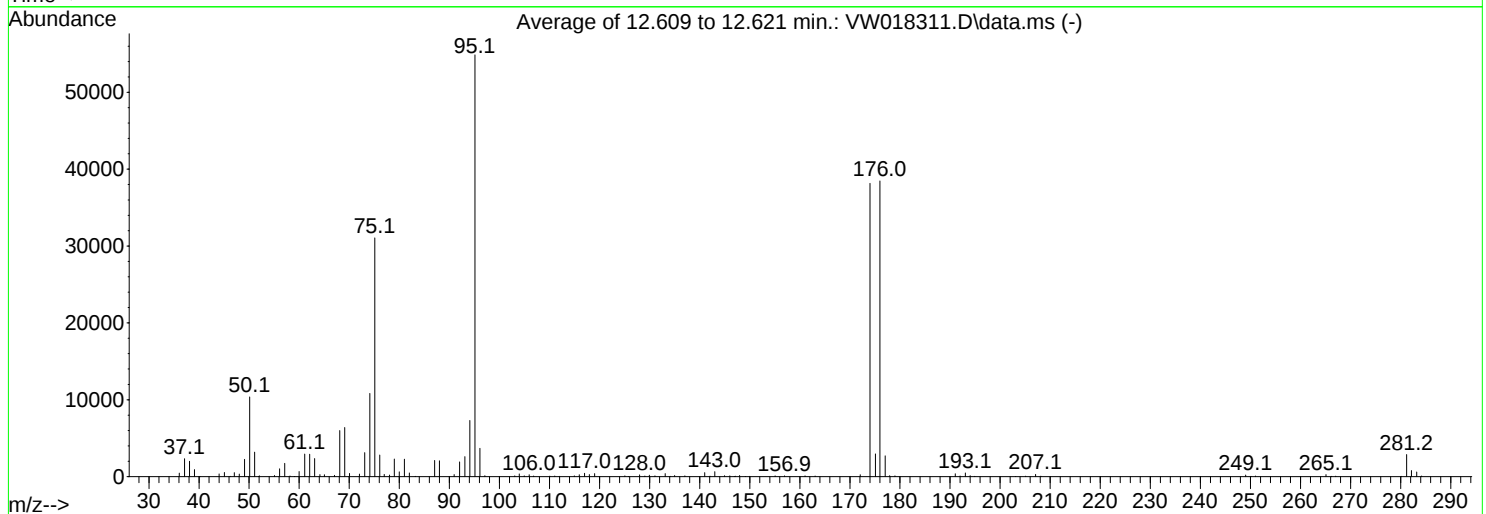


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031321\
Data File : VW018311.D
Acq On : 12 Mar 2021 10:50
Operator : SY/VA
Sample : BFB14
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB14

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Title : VOC Analysis
Last Update : Sat Mar 13 00:38:12 2021

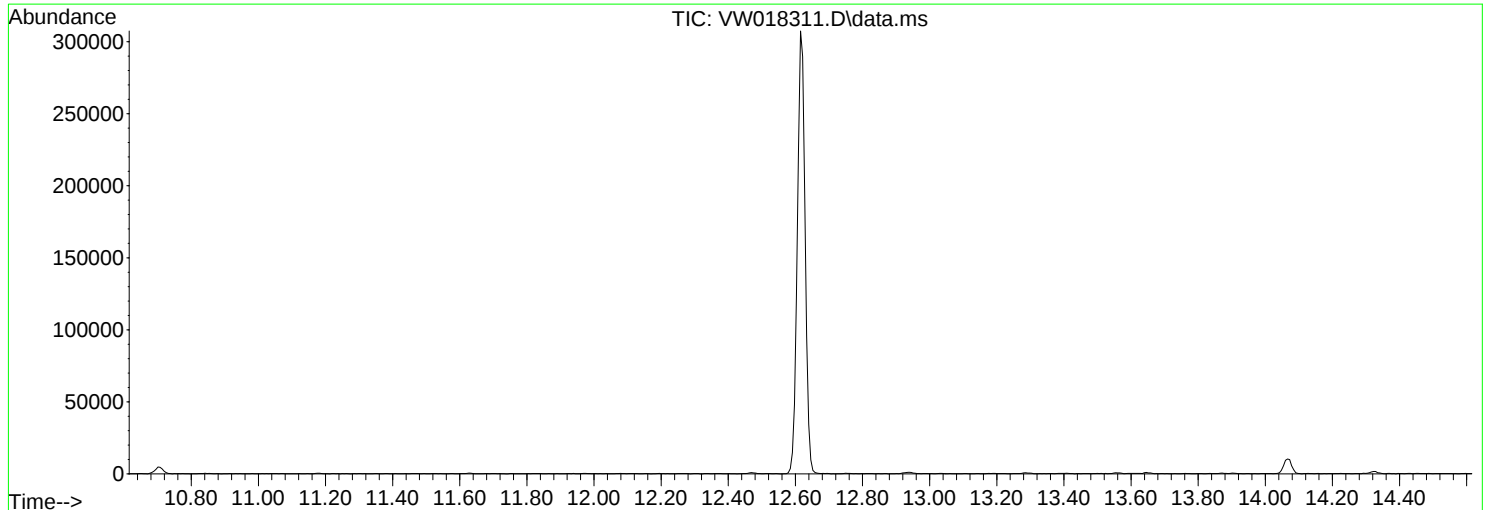

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	10361	PASS
75	95	30	80	56.6	31056	PASS
95	95	100	100	100.0	54872	PASS
96	95	5	9	6.7	3684	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.5	38157	PASS
175	174	5	9	7.7	2947	PASS
176	174	95	101	100.8	38472	PASS
177	176	5	9	7.1	2716	PASS

m/z	Abundance
36.00	423.0
37.10	2210.0
38.10	1871.0
39.10	813.0
40.10	88.0
44.10	379.0
45.00	524.0
47.10	375.0
48.10	263.0
49.10	1944.0
50.10	9075.0
51.10	2377.0
51.90	130.0
55.00	135.0
56.10	883.0
57.10	1454.0
58.20	84.0
59.10	71.0
60.00	567.0
61.10	2438.0
62.10	2422.0
63.10	2101.0
64.20	227.0
65.20	255.0
67.00	162.0
68.10	4842.0
69.10	5289.0
70.00	335.0
72.00	285.0
73.10	2793.0
74.10	9075.0
75.10	25960.0
76.10	2427.0
77.00	225.0
78.10	160.0
79.00	1862.0
80.00	556.0
81.00	1856.0
82.00	314.0
83.20	59.0
87.00	1785.0
88.00	1632.0
91.00	137.0
92.00	1541.0
93.10	2317.0
94.10	6211.0
95.10	43280.0
96.10	3301.0
97.00	115.0
103.00	177.0
104.00	346.0
105.00	142.0
105.90	204.0
106.80	63.0
110.00	53.0
111.00	78.0
112.00	105.0
115.00	101.0
116.00	264.0
117.00	472.0
118.00	221.0
119.00	375.0
125.20	110.0
128.00	196.0
129.00	75.0
130.00	162.0
131.00	91.0
133.10	617.0
134.10	81.0
135.00	152.0
137.20	52.0
141.00	349.0
143.00	483.0
145.00	78.0
146.00	60.0
146.90	50.0
147.90	93.0
149.10	51.0
149.90	74.0
155.10	53.0
157.00	83.0
161.00	97.0
163.00	154.0
172.00	194.0
174.00	28048.0
175.10	2435.0
176.00	29224.0
177.00	2304.0
177.90	88.0
179.00	172.0
191.10	537.0
192.00	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

193.00	609.0
194.10	146.0
195.00	96.0
205.10	76.0
207.10	290.0
208.20	148.0
249.10	241.0
250.10	98.0
251.00	155.0
265.10	301.0
266.20	55.0
280.10	117.0
281.20	3396.0
282.10	983.0
283.20	973.0
284.20	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

m/z	Abundance
36.10	553.0
37.10	2337.0
38.10	2090.0
39.10	1025.0
40.10	127.0
44.10	493.0
45.10	601.0
46.20	86.0
47.00	555.0
48.10	349.0
49.10	2352.0
50.10	12075.0
51.10	3665.0
52.10	149.0
55.10	201.0
56.10	1137.0
57.10	2015.0
58.10	61.0
60.00	763.0
61.10	3161.0
62.10	3171.0
63.10	2484.0
64.10	284.0
65.00	246.0
67.10	174.0
68.10	6516.0
69.10	7182.0
70.10	456.0
72.00	370.0
73.10	3449.0
74.10	12235.0
75.10	35200.0
76.10	3354.0
77.00	382.0
78.00	225.0
79.00	2561.0
80.00	760.0
81.00	2432.0
82.00	605.0
83.20	83.0
87.10	2155.0
88.00	2424.0
90.90	330.0
92.10	2123.0
93.10	2657.0
94.10	7720.0
95.10	62480.0
96.10	4238.0
97.10	150.0
103.10	154.0
103.90	368.0
104.90	94.0
106.00	289.0
106.90	80.0
110.10	66.0
111.00	67.0
111.80	54.0
114.90	120.0
115.90	276.0
117.00	408.0
117.90	353.0
119.00	322.0
125.00	231.0
125.80	51.0
128.00	260.0
129.00	77.0
129.80	176.0
131.00	100.0
133.10	405.0
134.10	70.0
135.00	157.0
137.10	81.0
141.00	598.0
142.00	91.0
143.00	773.0
144.90	196.0
146.00	118.0
147.10	116.0
148.00	176.0
155.10	95.0
156.90	108.0
161.10	124.0
163.10	78.0
172.10	310.0
174.00	43944.0
175.10	2932.0
176.00	42440.0
177.10	2801.0
178.00	169.0
179.00	94.0
191.00	355.0
192.00	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

193.10	487.0
194.00	120.0
194.90	56.0
203.10	54.0
205.10	124.0
207.00	377.0
208.10	67.0
249.00	266.0
251.00	70.0
265.10	362.0
266.20	52.0
267.10	123.0
281.20	3725.0
282.20	738.0
283.20	643.0
284.20	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

m/z	Abundance
36.10	377.0
37.10	2465.0
38.10	2036.0
39.10	904.0
40.00	120.0
44.00	416.0
45.10	508.0
46.20	65.0
47.10	615.0
48.00	399.0
49.10	2423.0
50.10	9934.0
51.10	3506.0
52.00	171.0
55.10	134.0
56.10	1056.0
57.10	1736.0
58.10	96.0
60.00	665.0
61.10	3223.0
62.10	3152.0
63.10	2471.0
64.10	281.0
65.00	243.0
67.10	167.0
68.10	6644.0
69.10	6679.0
70.10	439.0
72.10	366.0
73.10	3117.0
74.10	11177.0
75.10	32008.0
76.10	2665.0
77.00	268.0
78.00	217.0
79.00	2477.0
80.00	544.0
81.00	2525.0
82.00	511.0
87.00	2384.0
88.00	2143.0
90.90	374.0
92.10	2095.0
93.10	2834.0
94.10	7963.0
95.10	58856.0
96.10	3513.0
97.20	140.0
104.00	330.0
105.00	60.0
106.00	258.0
106.90	88.0
110.10	56.0
111.10	101.0
115.00	85.0
116.00	205.0
117.00	448.0
117.90	243.0
119.00	469.0
128.00	240.0
129.10	130.0
130.00	231.0
131.10	111.0
133.10	141.0
135.00	112.0
137.00	156.0
141.00	639.0
142.10	103.0
143.00	715.0
144.90	83.0
146.00	145.0
147.10	54.0
147.90	156.0
150.00	82.0
155.00	145.0
157.00	136.0
161.00	84.0
172.00	266.0
174.00	42480.0
175.10	3475.0
176.00	43752.0
177.10	3043.0
178.00	98.0
178.90	65.0
191.00	254.0
193.00	314.0
193.90	105.0
207.20	234.0
249.10	121.0
265.10	160.0
267.00	68.0
281.20	1480.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

282.20

283.10

284.20

624.0

201.0

56.0

Instrument :

MSVOA_W

ClientSampleId :

BFB14

m/z	Abundance
40.00	103.0
44.00	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14