


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031421\
Data File : VW018321.D
Acq On : 12 Mar 2021 16:03
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W031421S.M
Title : SW846 8260
Last Update : Sat Mar 13 04:56:13 2021

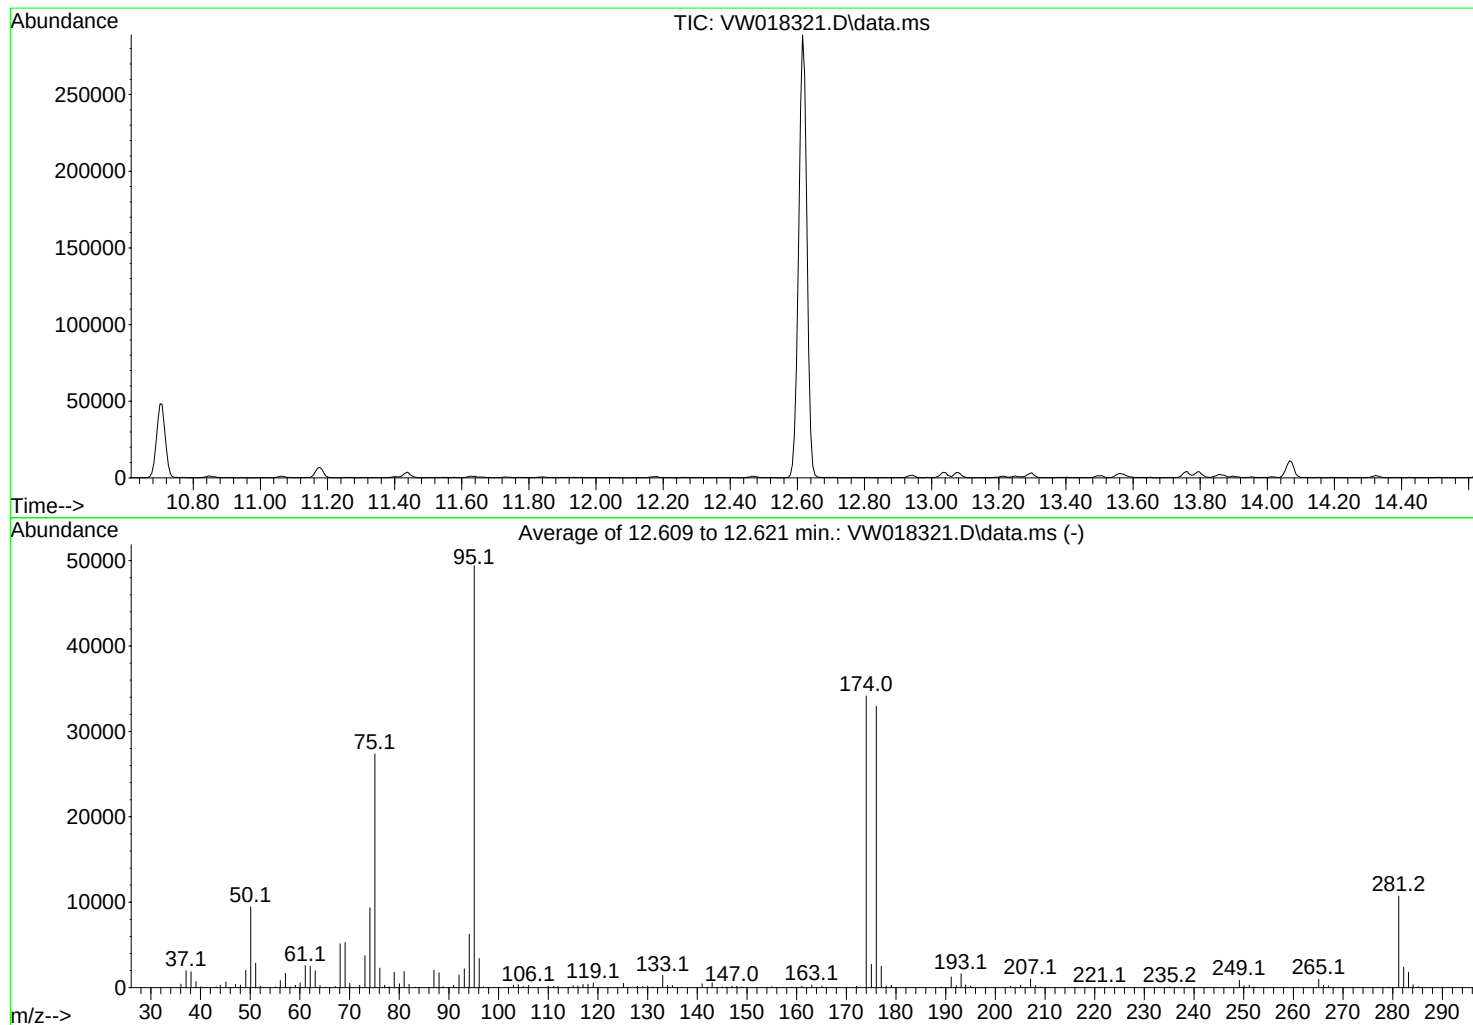

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	9455	PASS
75	95	30	60	55.4	27357	PASS
95	95	100	100	100.0	49387	PASS
96	95	5	9	6.9	3411	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.1	34149	PASS
175	174	5	9	8.0	2741	PASS
176	174	95	101	96.5	32963	PASS
177	176	5	9	7.6	2513	PASS