




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
Data File : VW022317.D
Acq On : 14 Mar 2022 13:59
Operator : SY/VA
Sample : N1820-03
Misc : 7.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRZ5

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:05:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 15 01:03:29 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
Supervised By :Mahesh Dadoda 03/15/2022

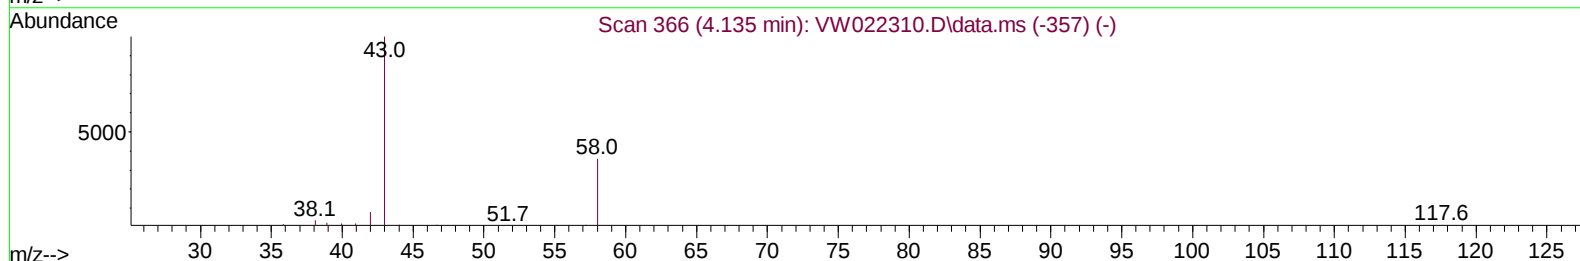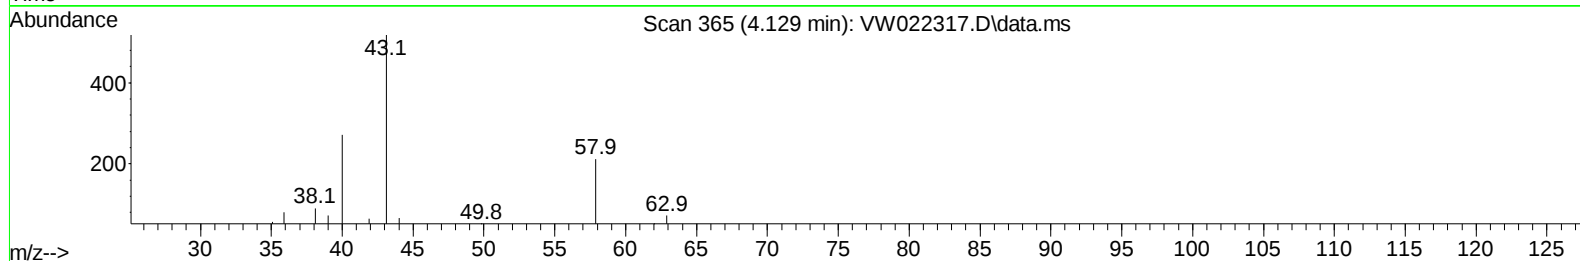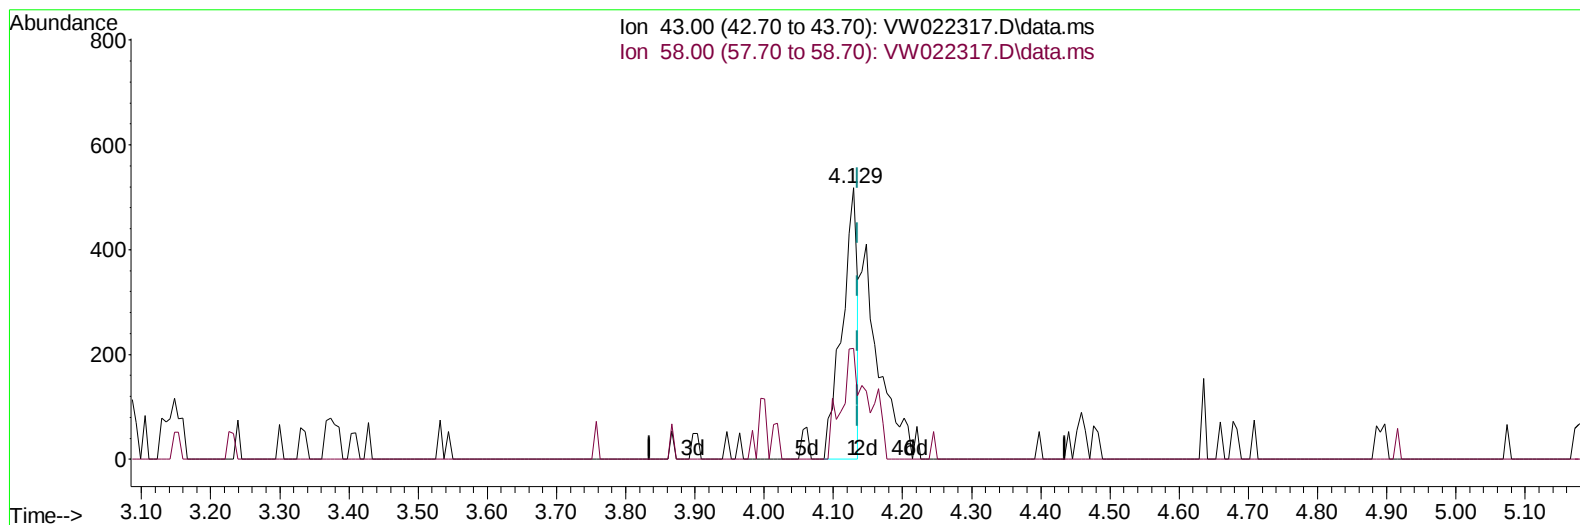

TIC: VW022317.D\data.ms

(13) Acetone (T)

4.129min (-0.006) 3.27 ug/L

response 799

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	34.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022317.D
 Acq On : 14 Mar 2022 13:59
 Operator : SY/VA
 Sample : N1820-03
 Misc : 7.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ5

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:05:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

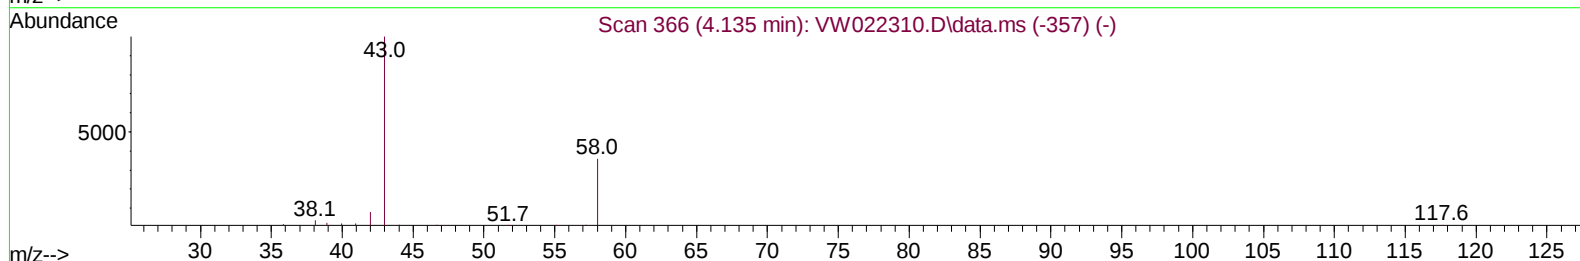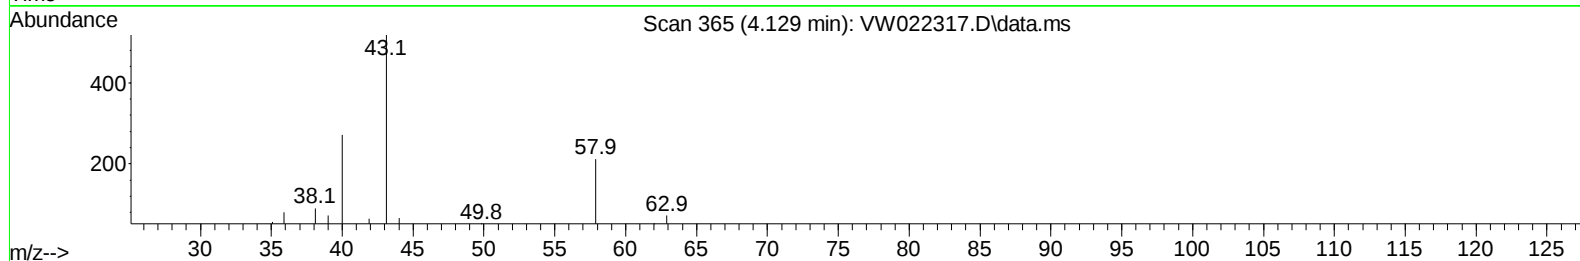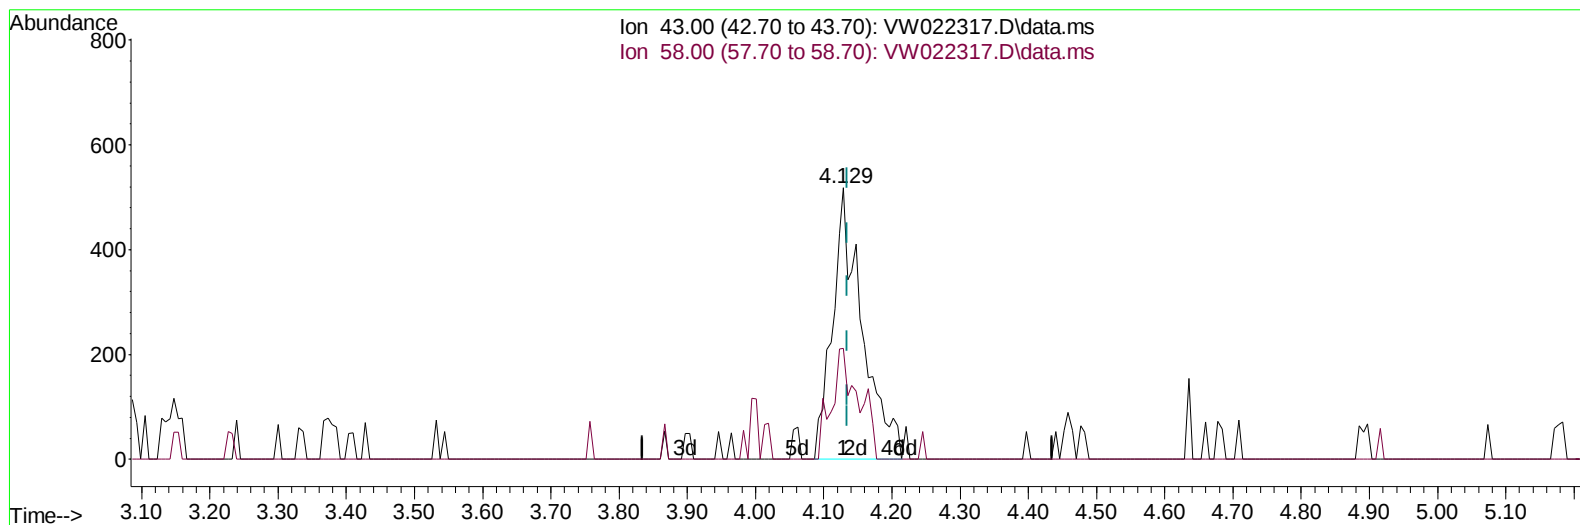

TIC: VW022317.D\data.ms

(13) Acetone (T)

4.129min (-0.006) 6.39 ug/L m

response 1562

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	17.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022317.D
 Acq On : 14 Mar 2022 13:59
 Operator : SY/VA
 Sample : N1820-03
 Misc : 7.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ5

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:05:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		136555	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		132733	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		65438	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		43210	24.260	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	97.040%		
7) Chloroethane-d5	2.879	69		29756	21.233	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	84.920%		
11) 1,1-Dichloroethene-d2	4.013	63		40679	14.914	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	59.640%		
21) 2-Butanone-d5	7.080	46		19151	63.951	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	127.900%		
24) Chloroform-d	7.647	84		72869	23.917	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	95.680%		
26) 1,2-Dichloroethane-d4	8.305	65		41331	26.097	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	104.400%		
32) Benzene-d6	8.275	84		134819	21.825	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.280%		
36) 1,2-Dichloropropane-d6	9.274	67		40767	23.764	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	95.040%		
41) Toluene-d8	10.323	98		125428	20.423	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.680%		
43) trans-1,3-Dichloroprop...	10.579	79		17676	23.238	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	92.960%		
47) 2-Hexanone-d5	10.920	63		15562	55.154	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	110.300%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		41302	27.433	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	109.720%		
66) 1,2-Dichlorobenzene-d4	13.853	152		54510	25.935	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	103.720%		
Target Compounds							
13) Acetone	4.129	43		1562m	6.386	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
Data File : VW022317.D
Acq On : 14 Mar 2022 13:59
Operator : SY/VA
Sample : N1820-03
Misc : 7.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRZ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/15/2022
Supervised By :Mahesh Dadoda 03/15/2022

Quant Time: Mar 15 01:05:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 15 01:03:29 2022
Response via : Initial Calibration

