




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022324.D
 Acq On : 14 Mar 2022 16:48
 Operator : SY/VA
 Sample : N1820-01
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ3

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:07:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

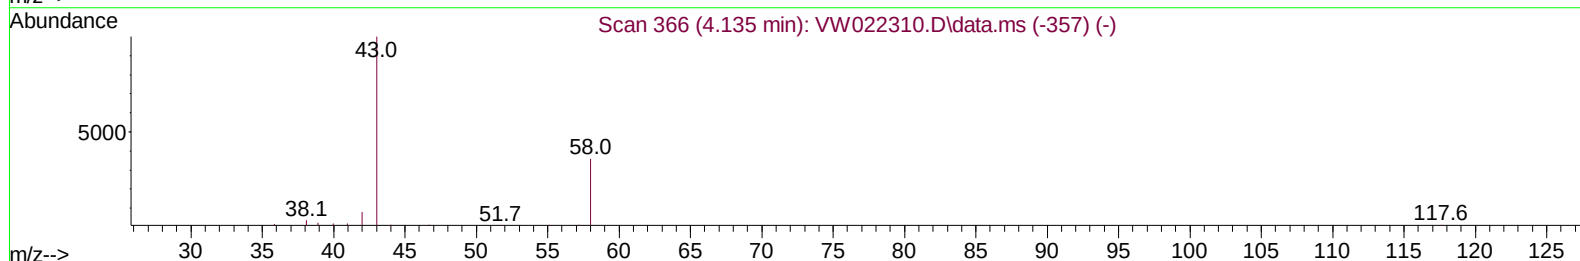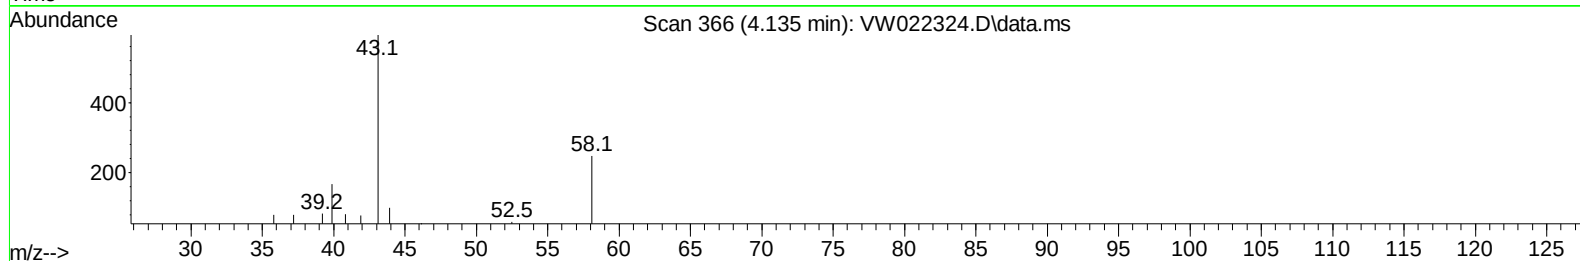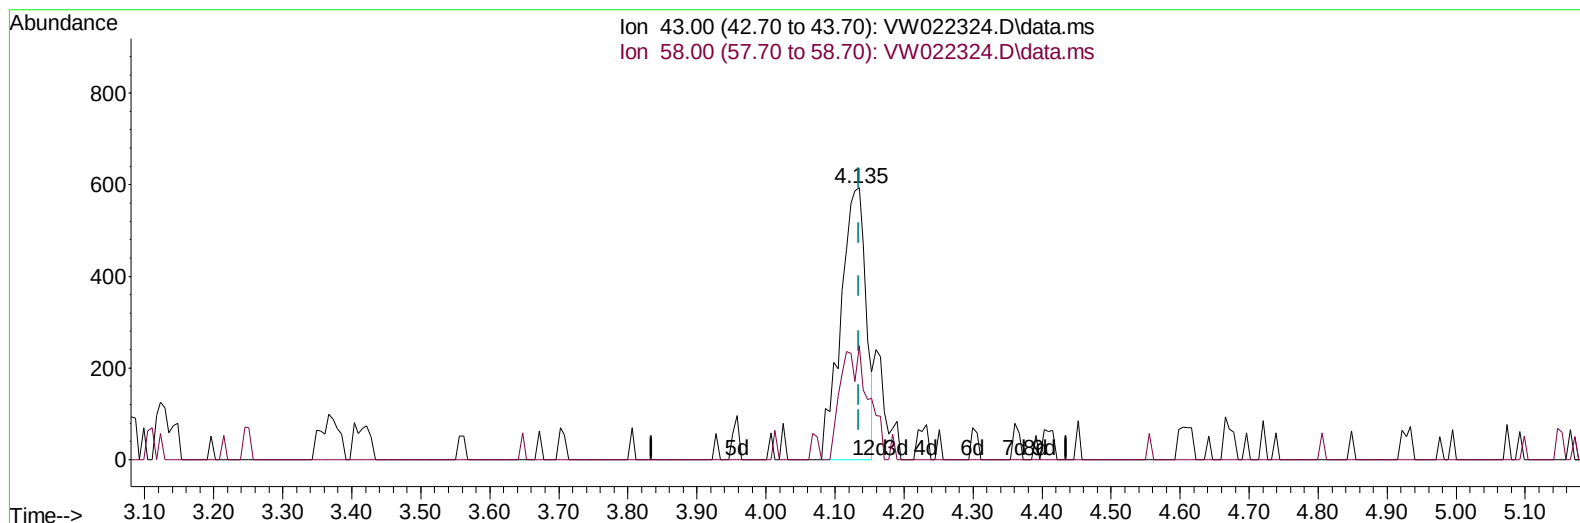

TIC: VW022324.D\data.ms

(13) Acetone (T)

4.135min (+ 0.000) 5.18 ug/L

response 1506

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	4.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022324.D
 Acq On : 14 Mar 2022 16:48
 Operator : SY/VA
 Sample : N1820-01
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ3

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:07:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

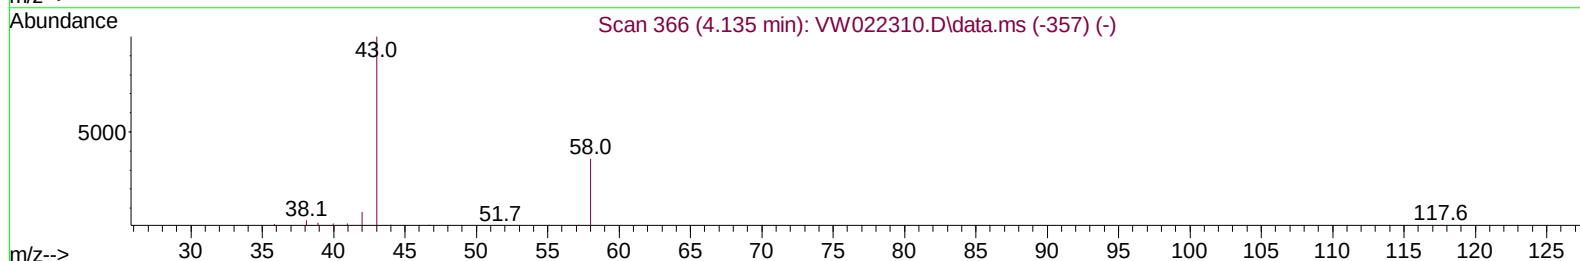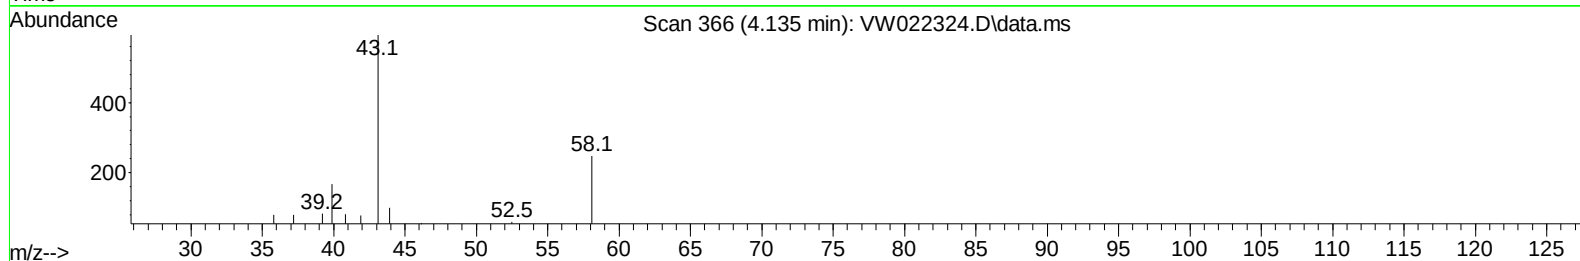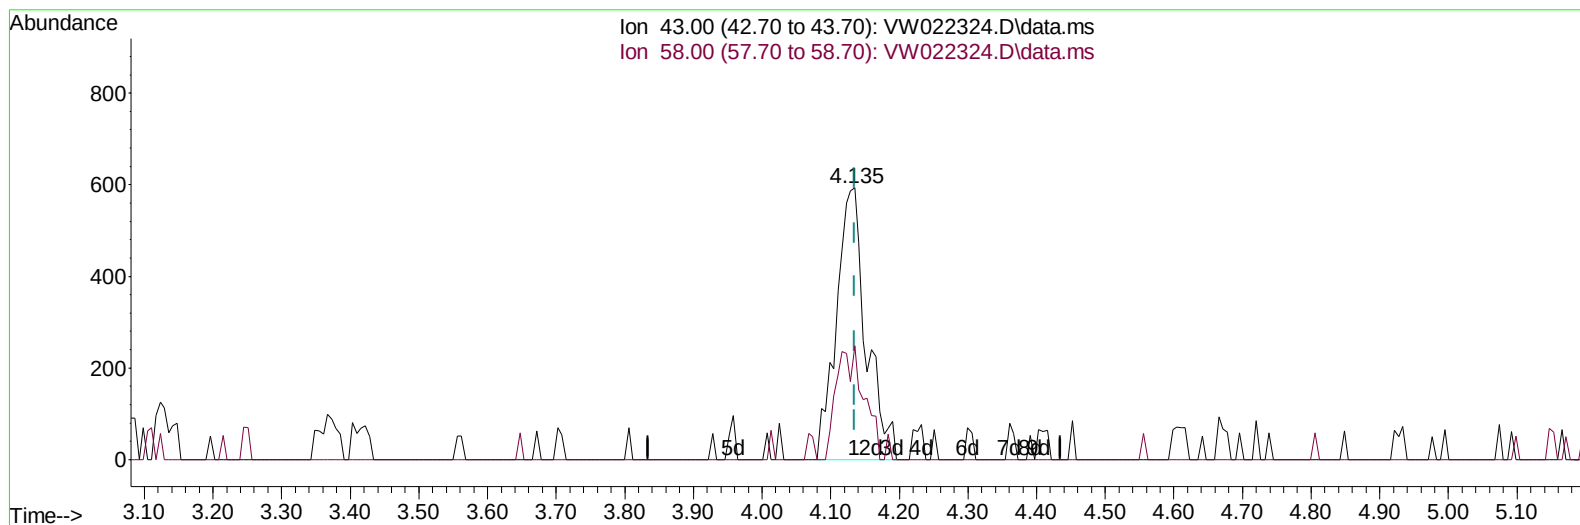

TIC: VW022324.D\data.ms

(13) Acetone (T)

4.135min (+ 0.000) 6.16 ug/L m

response 1790

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	3.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022324.D
 Acq On : 14 Mar 2022 16:48
 Operator : SY/VA
 Sample : N1820-01
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ3

Manual IntegrationsAPPROVED

Quant Time: Mar 15 01:07:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	162298	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	74367	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	44309	20.931	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.720%	
7) Chloroethane-d5	2.879	69	34640	20.798	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.200%	
11) 1,1-Dichloroethene-d2	4.007	63	41989	12.953	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.800%	
21) 2-Butanone-d5	7.080	46	18104	50.865	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.740%	
24) Chloroform-d	7.647	84	71841	19.840	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	79.360%	
26) 1,2-Dichloroethane-d4	8.305	65	38006	20.191	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	80.760%	
32) Benzene-d6	8.275	84	133365	18.841	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	75.360%	
36) 1,2-Dichloropropane-d6	9.274	67	38985	19.832	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	79.320%	
41) Toluene-d8	10.323	98	123757	17.586	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.360%	
43) trans-1,3-Dichloroprop...	10.573	79	15904	18.247	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	73.000%	
47) 2-Hexanone-d5	10.920	63	14035	43.410	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.820%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38000	22.027	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.120%	
66) 1,2-Dichlorobenzene-d4	13.847	152	48481	20.297	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	81.200%	
Target Compounds						
13) Acetone	4.135	43	1790m	6.158	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
Data File : VW022324.D
Acq On : 14 Mar 2022 16:48
Operator : SY/VA
Sample : N1820-01
Misc : 5.73g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRZ3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/15/2022
Supervised By :Mahesh Dadoda 03/15/2022

Quant Time: Mar 15 01:07:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 15 01:03:29 2022
Response via : Initial Calibration

