

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022314.D
 Acq On : 14 Mar 2022 12:28
 Operator : SY/VA
 Sample : N1820-09
 Misc : 5.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG0

Quant Time: Mar 15 01:04:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	149107	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	142825	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	68554	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	42723	21.968	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.880%
7) Chloroethane-d5	2.885	69	30924	20.209	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.840%
11) 1,1-Dichloroethene-d2	4.013	63	42376	14.229	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.920%
21) 2-Butanone-d5	7.092	46	15485	47.356	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.720%
24) Chloroform-d	7.647	84	76422	22.972	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.880%
26) 1,2-Dichloroethane-d4	8.305	65	40123	23.202	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	8.275	84	137205	20.641	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.560%
36) 1,2-Dichloropropane-d6	9.274	67	41754	22.619	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.480%
41) Toluene-d8	10.323	98	128914	19.508	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.040%
43) trans-1,3-Dichloroprop...	10.579	79	16954	20.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.840%
47) 2-Hexanone-d5	10.920	63	12691	41.801	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.600%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38408	23.708	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%
66) 1,2-Dichlorobenzene-d4	13.847	152	51537	23.406	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.640%
Target Compounds						
13) Acetone	4.141	43	3102	11.615	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
Data File : VW022314.D
Acq On : 14 Mar 2022 12:28
Operator : SY/VA
Sample : N1820-09
Misc : 5.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG0


Quant Time: Mar 15 01:04:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 15 01:03:29 2022
Response via : Initial Calibration

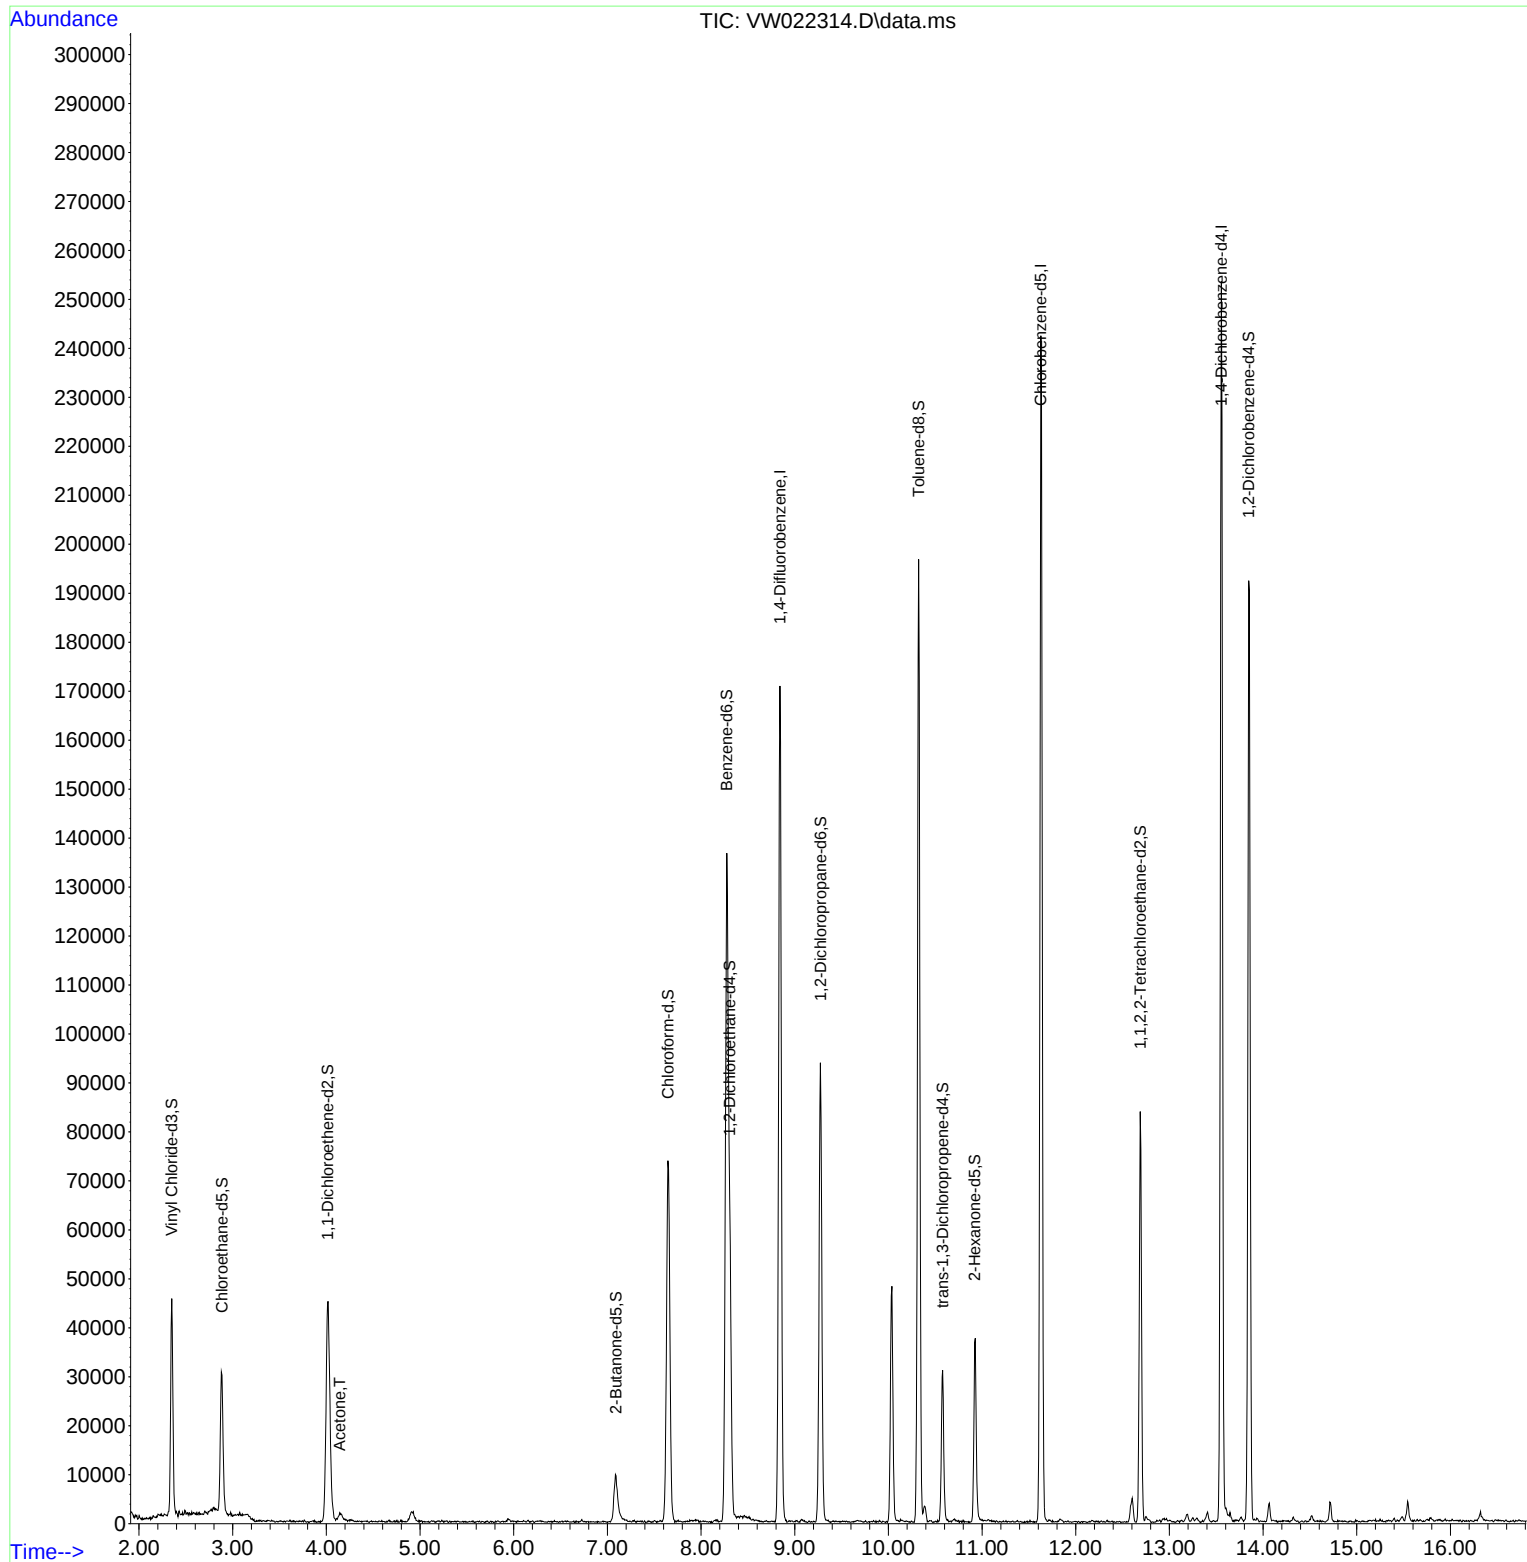

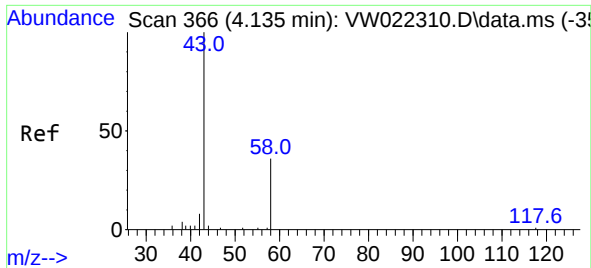

#13
 Acetone
 Concen: 11.615 ug/L
 RT: 4.141 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022314.D
 Acq: 14 Mar 2022 12:28

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG0

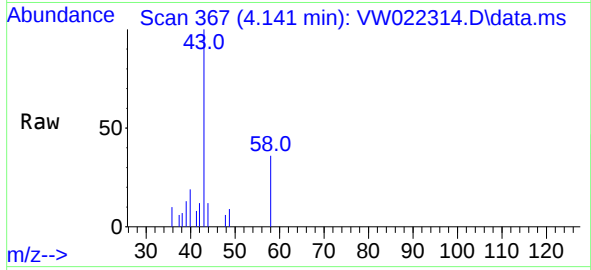

Tgt Ion: 43 Resp: 3102
 Ion Ratio Lower Upper
 43 100
 58 23.3 0.0 69.2

