

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
 Data File : VW022324.D
 Acq On : 14 Mar 2022 16:48
 Operator : SY/VA
 Sample : N1820-01
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRZ3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/15/2022
 Supervised By :Mahesh Dadoda 03/15/2022

Quant Time: Mar 15 01:07:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 15 01:03:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	162298	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	74367	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	44309	20.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.720%
7) Chloroethane-d5	2.879	69	34640	20.798	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.200%
11) 1,1-Dichloroethene-d2	4.007	63	41989	12.953	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.800%
21) 2-Butanone-d5	7.080	46	18104	50.865	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.740%
24) Chloroform-d	7.647	84	71841	19.840	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.360%
26) 1,2-Dichloroethane-d4	8.305	65	38006	20.191	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.760%
32) Benzene-d6	8.275	84	133365	18.841	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.360%
36) 1,2-Dichloropropane-d6	9.274	67	38985	19.832	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.320%
41) Toluene-d8	10.323	98	123757	17.586	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.360%
43) trans-1,3-Dichloroprop...	10.573	79	15904	18.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.000%
47) 2-Hexanone-d5	10.920	63	14035	43.410	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.820%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38000	22.027	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	48481	20.297	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.200%
Target Compounds					Qvalue	
13) Acetone	4.135	43	1790m	6.158	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031422\
Data File : VW022324.D
Acq On : 14 Mar 2022 16:48
Operator : SY/VA
Sample : N1820-01
Misc : 5.73g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRZ3

Quant Time: Mar 15 01:07:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 15 01:03:29 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/15/2022
Supervised By :Mahesh Dadoda 03/15/2022

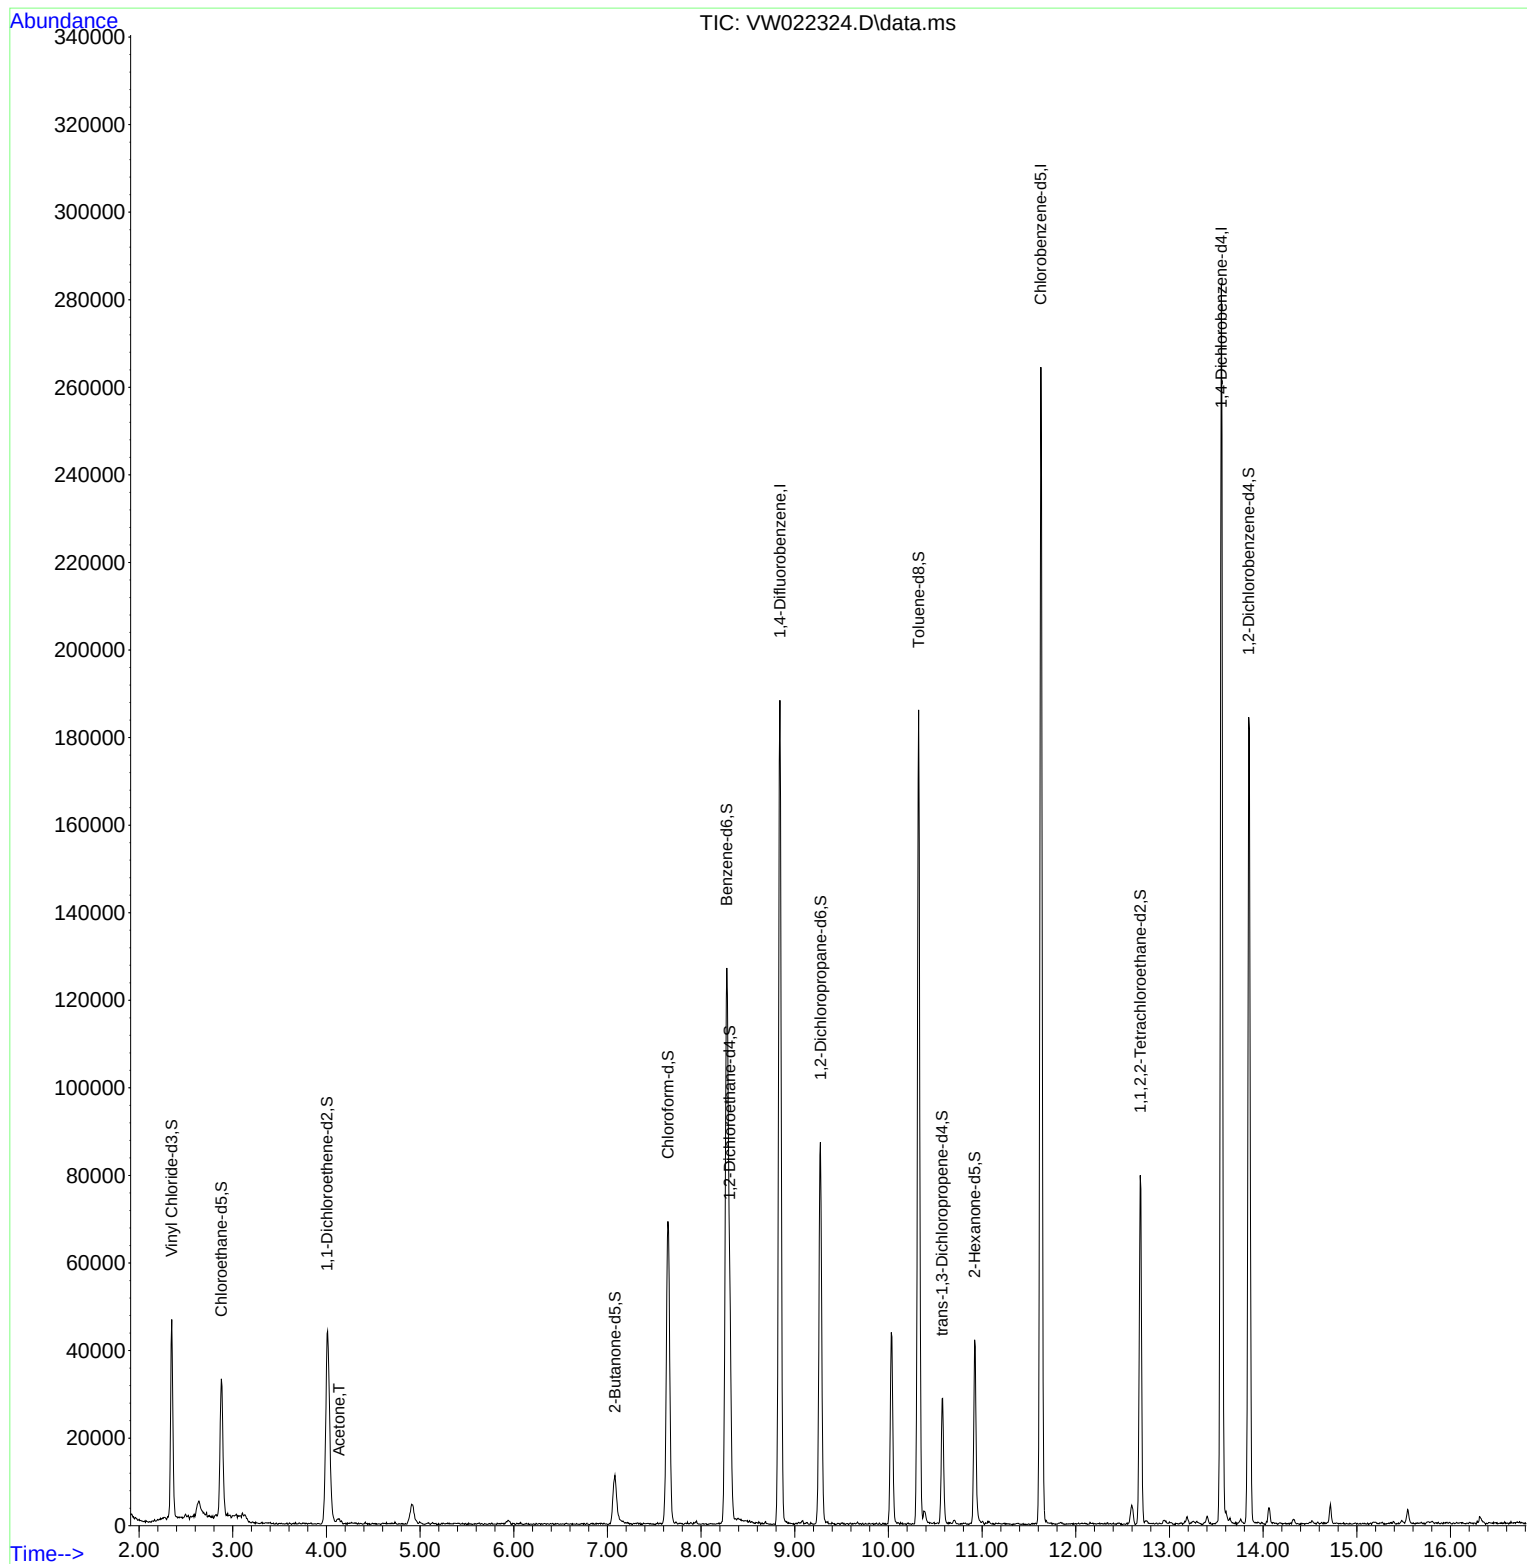

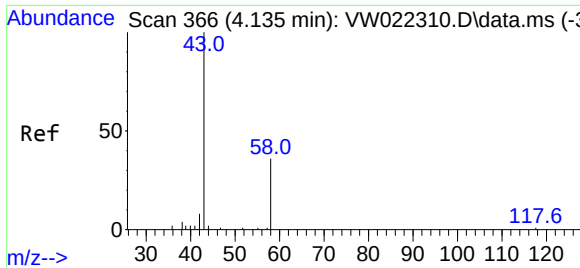

#13
Acetone
Concen: 6.158 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW022324.D
Acq: 14 Mar 2022 16:48

Instrument :
MSVOA_W
ClientSampleId :
DBRZ3

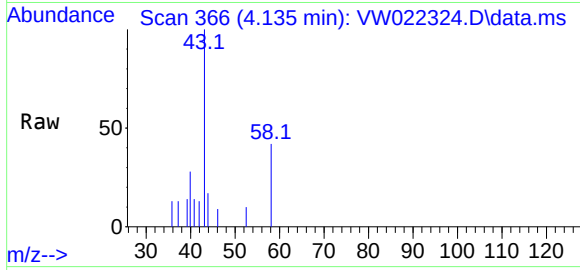

Tgt Ion: 43 Resp: 1790
Ion Ratio Lower Upper
43 100
58 3.7 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/15/2022
Supervised By :Mahesh Dadoda 03/15/2022

