

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW031519\
 Data File : VW009198.D
 Acq On : 15 Mar 2019 15:00
 Operator : SY/VA
 Sample : K1794-11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 3/16/2019 2:56:10 PM

Quant Time: Mar 15 23:41:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 23:26:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	441785	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	423688	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	201499	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	153536	29.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.32%
7) Chloroethane-d5	2.89	69	142917	23.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.56%
10) 1,1-Dichloroethene-d2	4.01	63	225014	19.72	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.88%
20) 2-Butanone-d5	7.07	46	105611	48.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.74%
24) Chloroform-d	7.65	84	297321	24.66	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.64%
26) 1,2-Dichloroethane-d4	8.30	65	184610	25.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.68%
29) Benzene-d6	8.27	84	583061	24.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.80%
33) 1,2-Dichloropropane-d6	9.27	67	173299	24.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.76%
37) Toluene-d8	10.32	98	536392	24.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.32%
38) trans-1,3-Dichloropropene-	10.58	79	82821	23.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.00%
39) 2-Hexanone-d5	10.93	63	80176	47.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	162268	23.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.92%
61) 1,2-Dichlorobenzene-d4	13.85	152	197811	25.60	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.40%

Target Compounds				Ovalue
16) Methylene chloride	4.92	84	10500m	1.630 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW031519\
Data File : VW009198.D
Acq On : 15 Mar 2019 15:00
Operator : SY/VA
Sample : K1794-11
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
3/16/2019 2:56:10 PM

Quant Time: Mar 15 23:41:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 23:26:07 2019
Response via : Initial Calibration

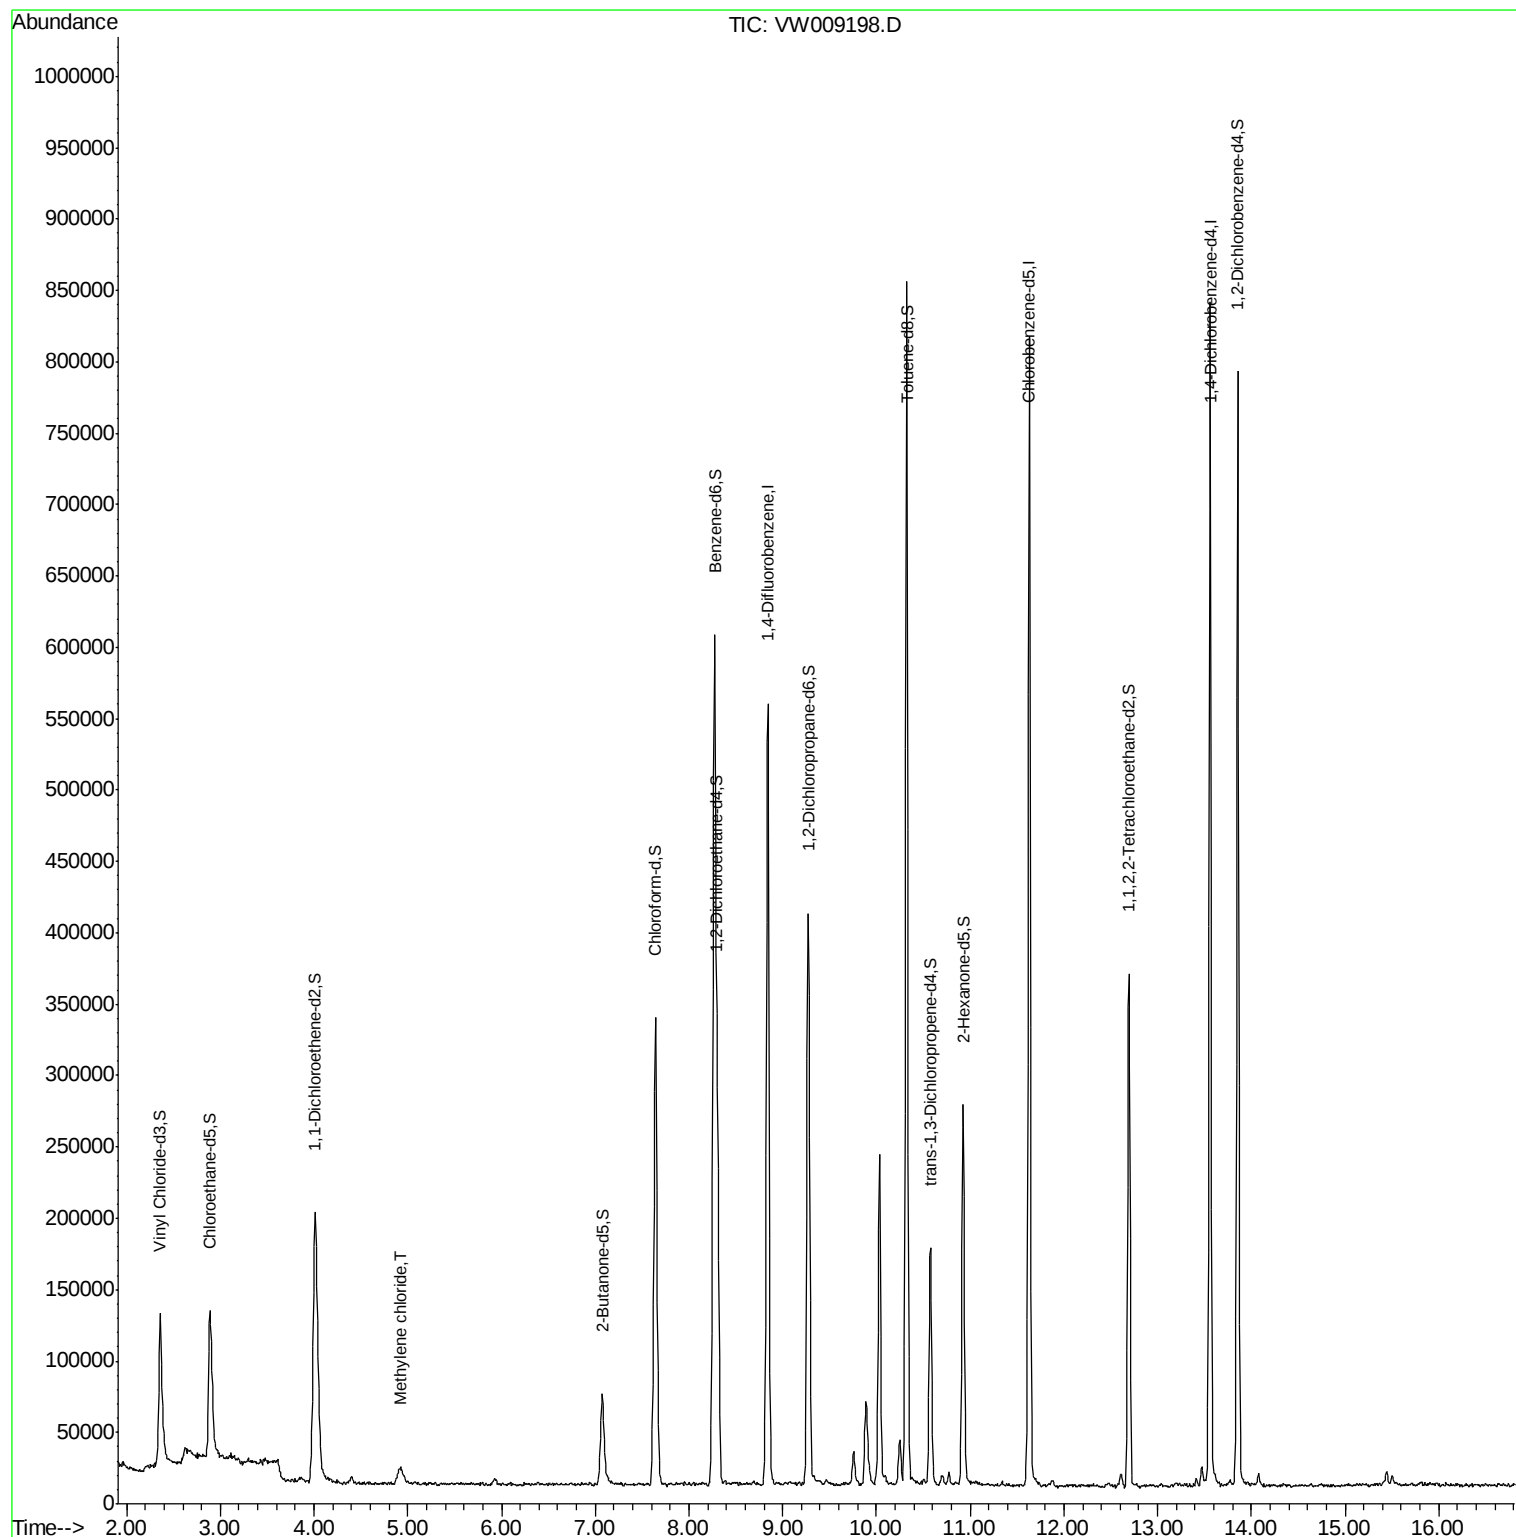

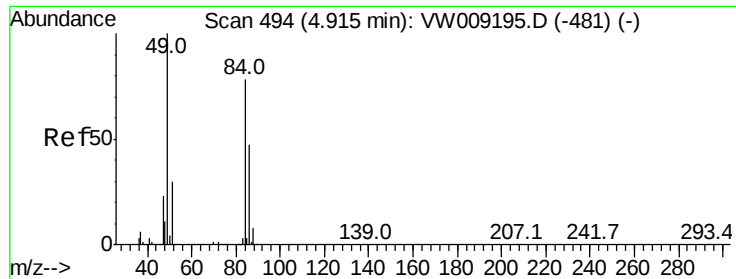

#16
 Methvlene chloride
 Concen: 1.630 ug/L m
 RT: 4.92 min Scan# 494
 Delta R.T. 0.00 min
 Lab File: VW009198.D
 Acq: 15 Mar 2019 15:00

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Tot Ion	Ratio	Lower	Upper
84	100		
49	150.5	96.0	178.2
86	48.6	44.4	82.5

Manual Integrations
 APPROVED

MMDadoda
 3/16/2019 2:56:10 PM

