

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031521\
 Data File : VW018338.D
 Acq On : 15 Mar 2021 12:55
 Operator : SY/VA
 Sample : VW0315SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK17

Quant Time: Mar 16 01:17:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 16 01:16:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	208203	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	190252	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	86711	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	53227	23.61	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.44%		
7) Chloroethane-d5	2.897	69	43688	23.86	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	95.44%		
10) 1,1-Dichloroethene-d2	4.025	63	94040	17.95	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.80%		
20) 2-Butanone-d5	7.080	46	27449	51.21	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.42%		
24) Chloroform-d	7.653	84	141014	25.00	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	100.00%		
26) 1,2-Dichloroethane-d4	8.305	65	78554	25.31	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.24%		
29) Benzene-d6	8.275	84	254376	25.12	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.48%		
33) 1,2-Dichloropropane-d6	9.274	67	71363	25.43	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.72%		
37) Toluene-d8	10.323	98	242068	24.77	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	99.08%		
38) trans-1,3-Dichloroprop...	10.579	79	32505	23.37	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	93.48%		
39) 2-Hexanone-d5	10.927	63	23427	50.18	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.36%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	59243	24.69	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.76%		
61) 1,2-Dichlorobenzene-d4	13.853	152	83966	26.64	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	106.56%		
Target Compounds						Qvalue
16) Methylene chloride	4.934	84	3596	1.13	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031521\
Data File : VW018338.D
Acq On : 15 Mar 2021 12:55
Operator : SY/VA
Sample : VW0315SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK17

Quant Time: Mar 16 01:17:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM030821S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 16 01:16:18 2021
Response via : Initial Calibration

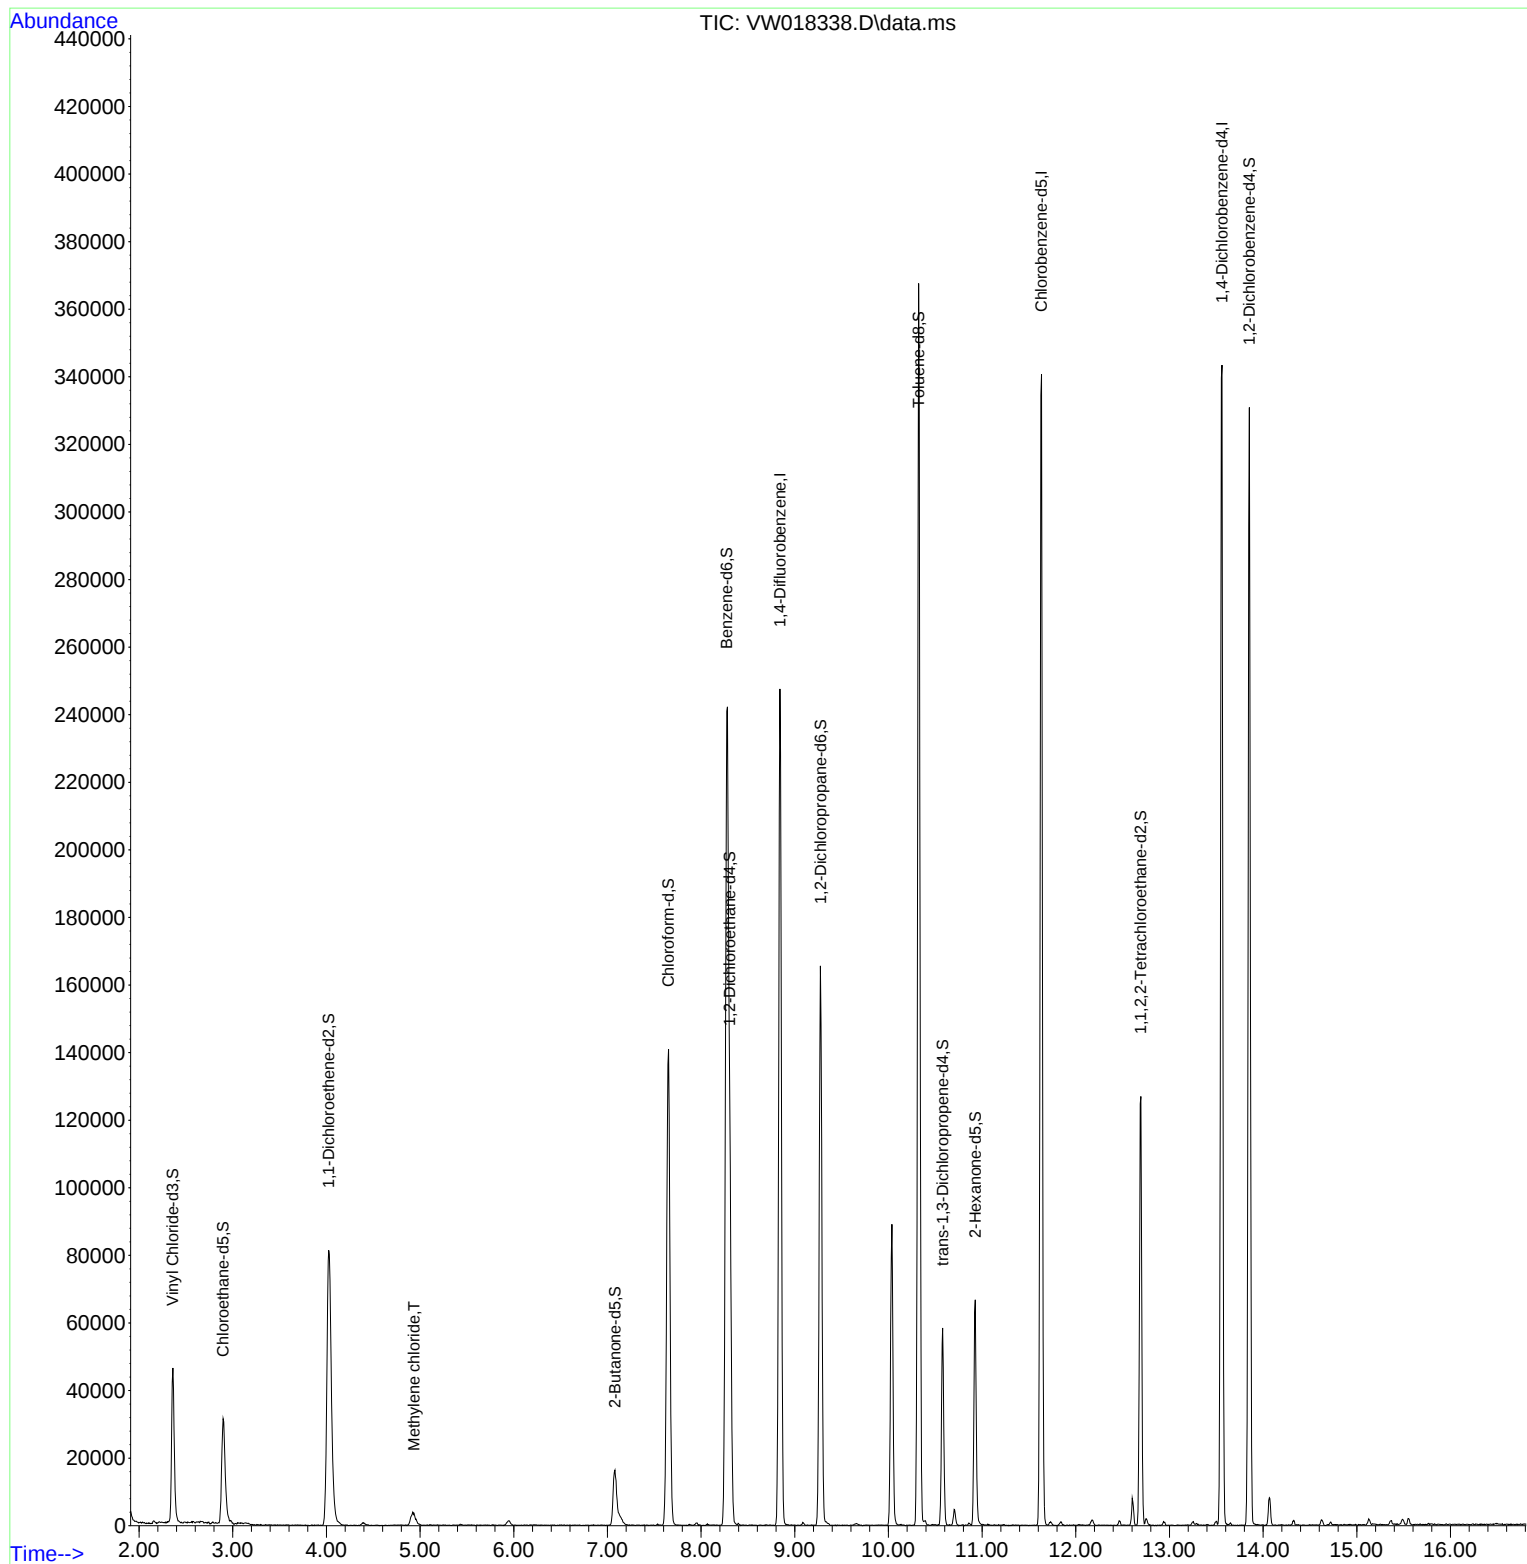

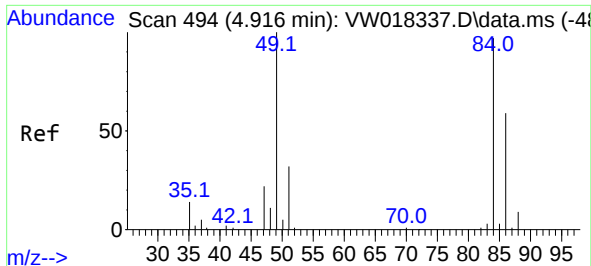

#16
Methylene chloride
Concen: 1.13 ug/L
RT: 4.934 min Scan# 497
Delta R.T. 0.018 min
Lab File: VW018338.D
Acq: 15 Mar 2021 12:55

Instrument :
MSVOA_W
ClientSampleId :
VBLK17

Tgt Ion: 84 Resp: 3596

Ion	Ratio	Lower	Upper
84	100		
49	102.1	74.4	138.2
86	71.3	46.1	85.7

