

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022343.D
 Acq On : 15 Mar 2022 17:35
 Operator : SY/VA
 Sample : N1883-04RE
 Misc : 5.50g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA3

Quant Time: Mar 16 05:36:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	181523	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	170478	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	85049	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	45804	19.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.400%
7) Chloroethane-d5	2.885	69	37315	20.031	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.120%
11) 1,1-Dichloroethene-d2	4.013	63	52530	14.488	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.960%
21) 2-Butanone-d5	7.080	46	23594	59.269	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.540%
24) Chloroform-d	7.653	84	93049	22.975	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.880%
26) 1,2-Dichloroethane-d4	8.305	65	50438	23.958	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.840%
32) Benzene-d6	8.275	84	174975	22.054	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.200%
36) 1,2-Dichloropropane-d6	9.275	67	51002	23.147	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.600%
41) Toluene-d8	10.323	98	160675	20.370	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.480%
43) trans-1,3-Dichloroprop...	10.579	79	22127	22.649	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.600%
47) 2-Hexanone-d5	10.921	63	18846	52.005	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.000%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	50209	25.965	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	66918	24.497	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.000%
Target Compounds						
39) cis-1,3-Dichloropropene	10.037	75	1817	0.622	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022343.D
Acq On : 15 Mar 2022 17:35
Operator : SY/VA
Sample : N1883-04RE
Misc : 5.50g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSA3

Quant Time: Mar 16 05:36:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

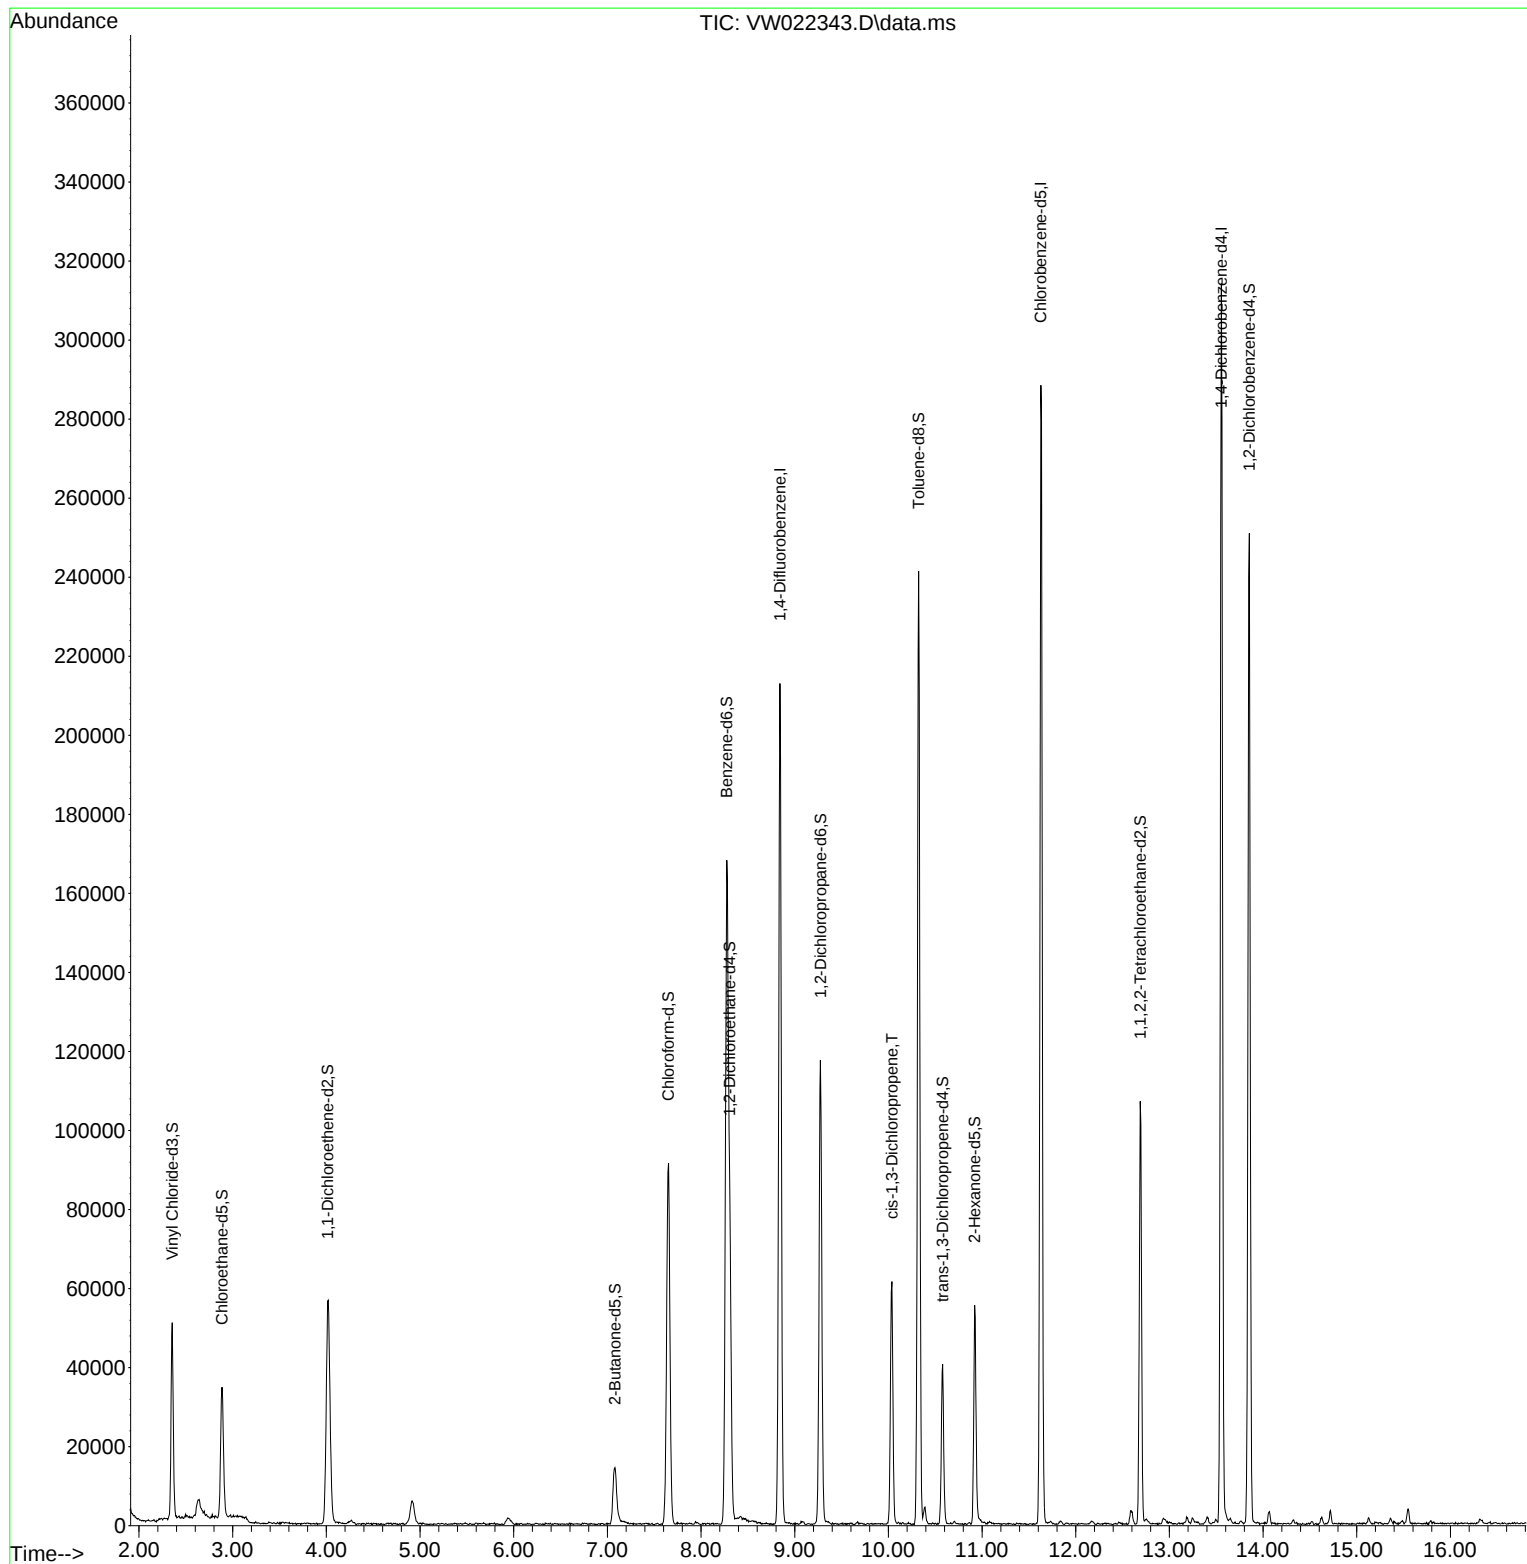

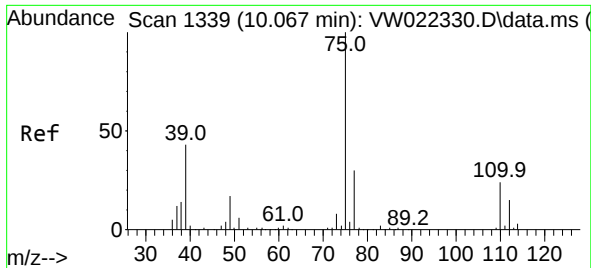

#39
 cis-1,3-Dichloropropene
 Concen: 0.622 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW022343.D
 Acq: 15 Mar 2022 17:35

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA3

Tgt Ion: 75 Resp: 1817
 Ion Ratio Lower Upper
 75 100
 77 47.5 20.6 38.2#

