




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022332.D
Acq On : 15 Mar 2022 13:11
Operator : SY/VA
Sample : N1820-09
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:34:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

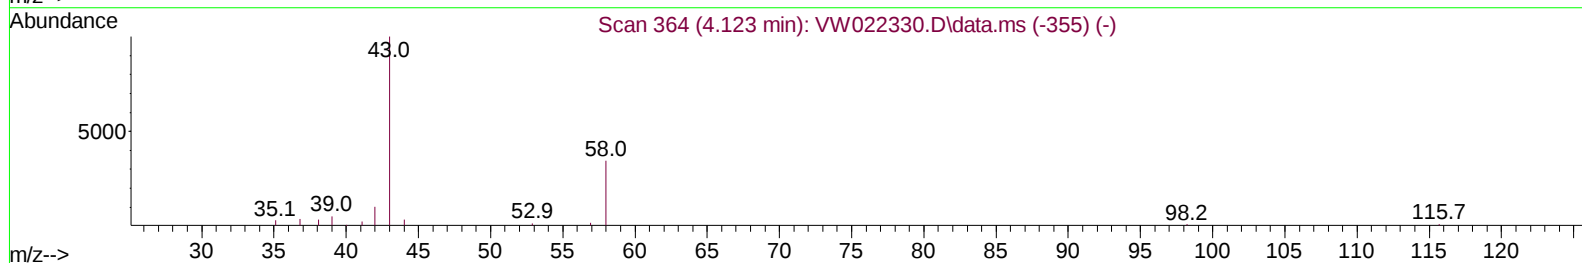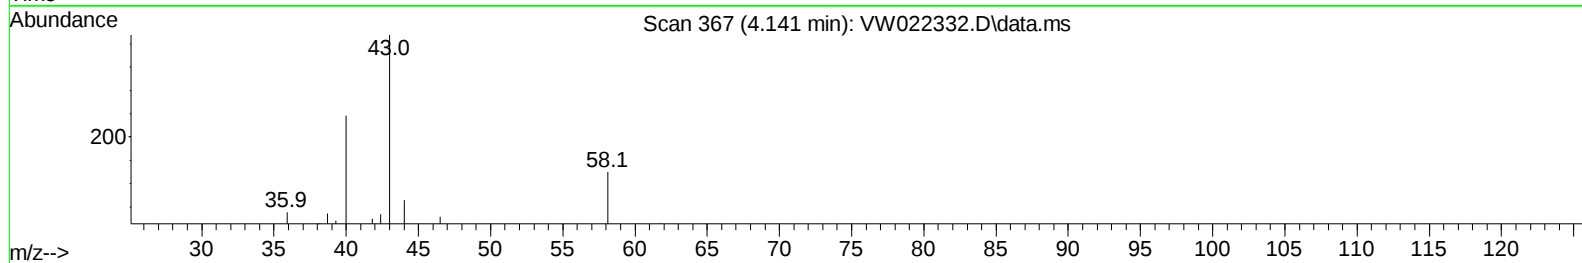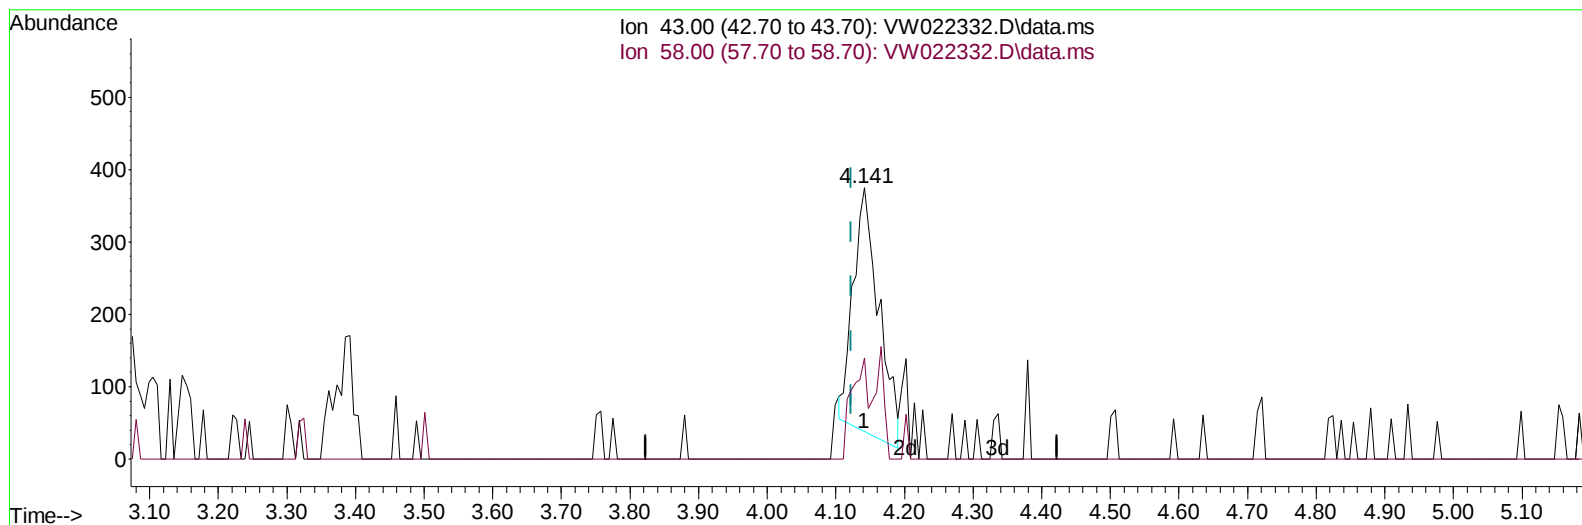

TIC: VW022332.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 3.14 ug/L

response 866

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	25.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022332.D
Acq On : 15 Mar 2022 13:11
Operator : SY/VA
Sample : N1820-09
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:34:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

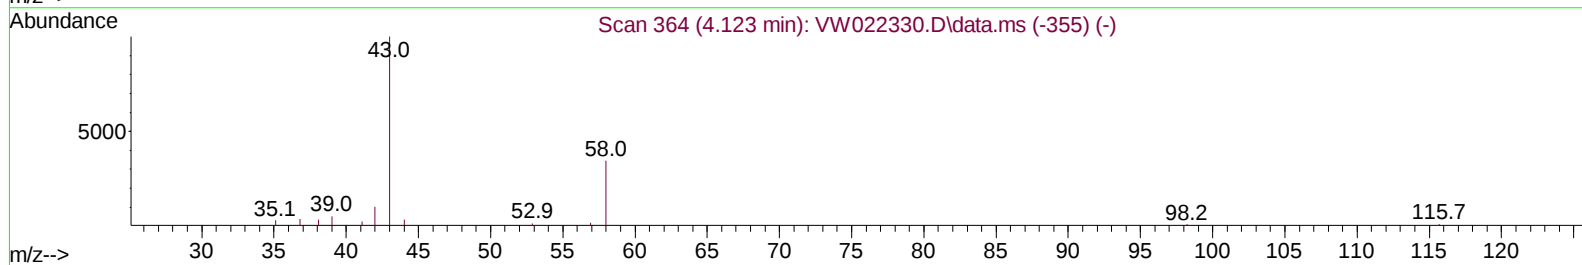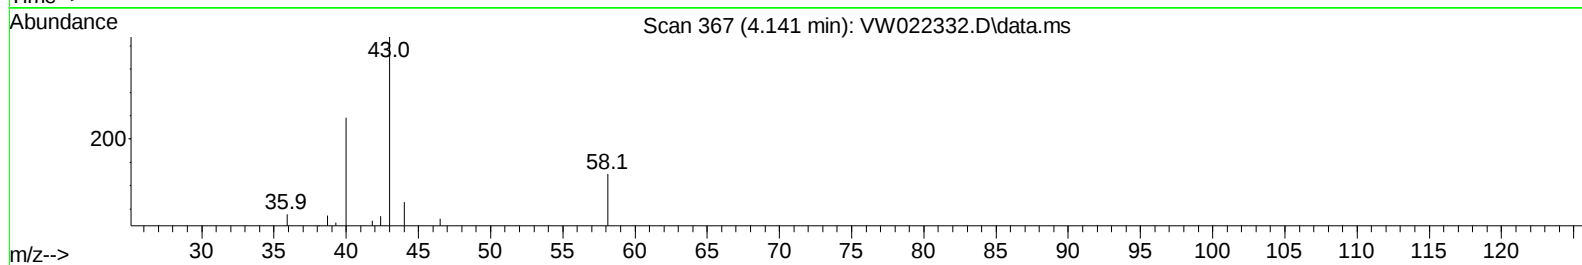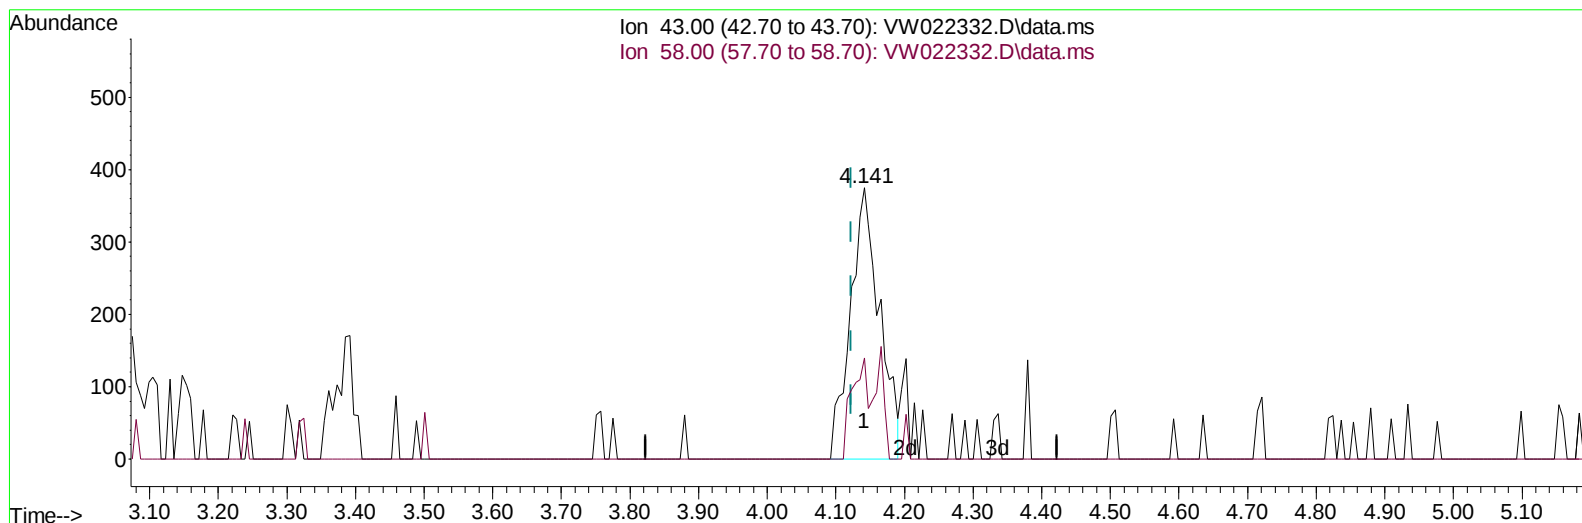

TIC: VW022332.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 4.01 ug/L m

response 1107

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	19.96
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022332.D
 Acq On : 15 Mar 2022 13:11
 Operator : SY/VA
 Sample : N1820-09
 Misc : 5.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:34:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	154192	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	149889	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	71559	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	42914	21.338	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	85.360%		
7) Chloroethane-d5	2.879	69	33601	21.234	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	84.920%		
11) 1,1-Dichloroethene-d2	4.013	63	39785	12.918	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	51.680%		
21) 2-Butanone-d5	7.080	46	17130	50.659	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	101.320%		
24) Chloroform-d	7.653	84	73555	21.381	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	85.520%		
26) 1,2-Dichloroethane-d4	8.305	65	39549	22.116	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	88.480%		
32) Benzene-d6	8.275	84	133992	19.208	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	76.840%		
36) 1,2-Dichloropropane-d6	9.268	67	40121	20.710	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	82.840%		
41) Toluene-d8	10.323	98	122612	17.680	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	70.720%		
43) trans-1,3-Dichloroprop...	10.573	79	16420	19.116	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	76.480%		
47) 2-Hexanone-d5	10.921	63	13828	43.399	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	86.800%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40052	23.558	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	94.240%		
66) 1,2-Dichlorobenzene-d4	13.847	152	53042	23.078	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	92.320%		
Target Compounds						
13) Acetone	4.141	43	1107m	4.008	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022332.D
Acq On : 15 Mar 2022 13:11
Operator : SY/VA
Sample : N1820-09
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:34:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

