




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022339.D
Acq On : 15 Mar 2022 15:59
Operator : SY/VA
Sample : N1883-16
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB3

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:35:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

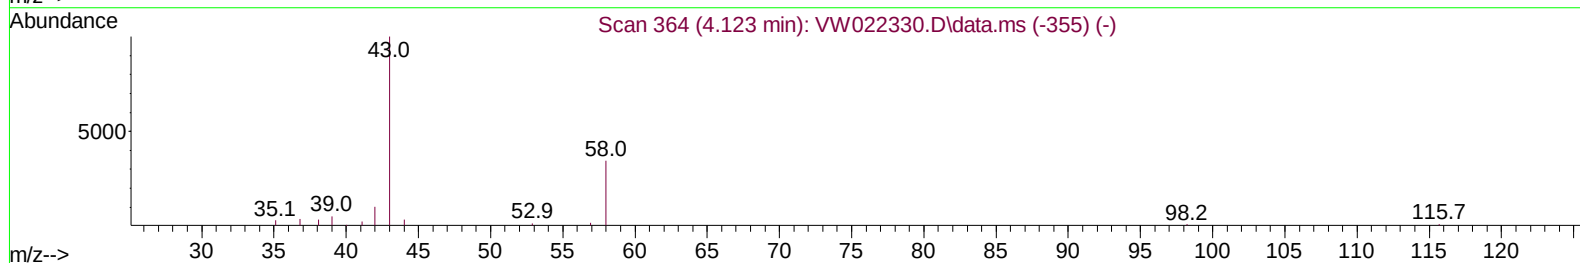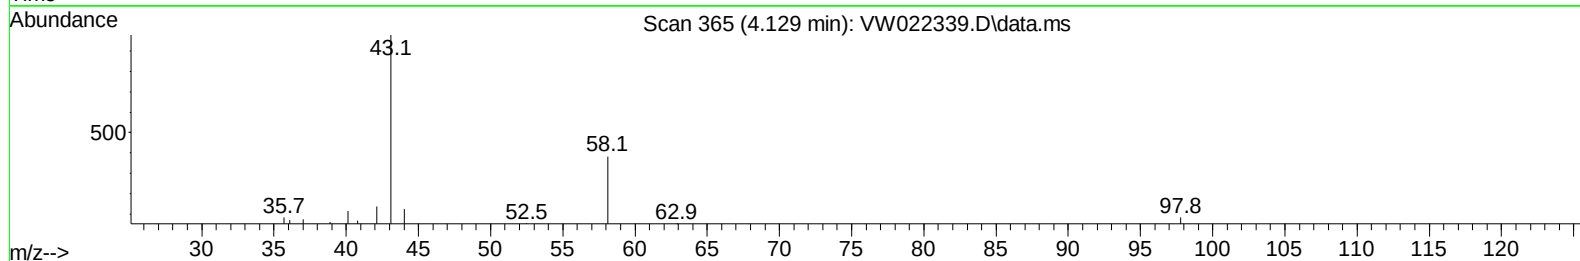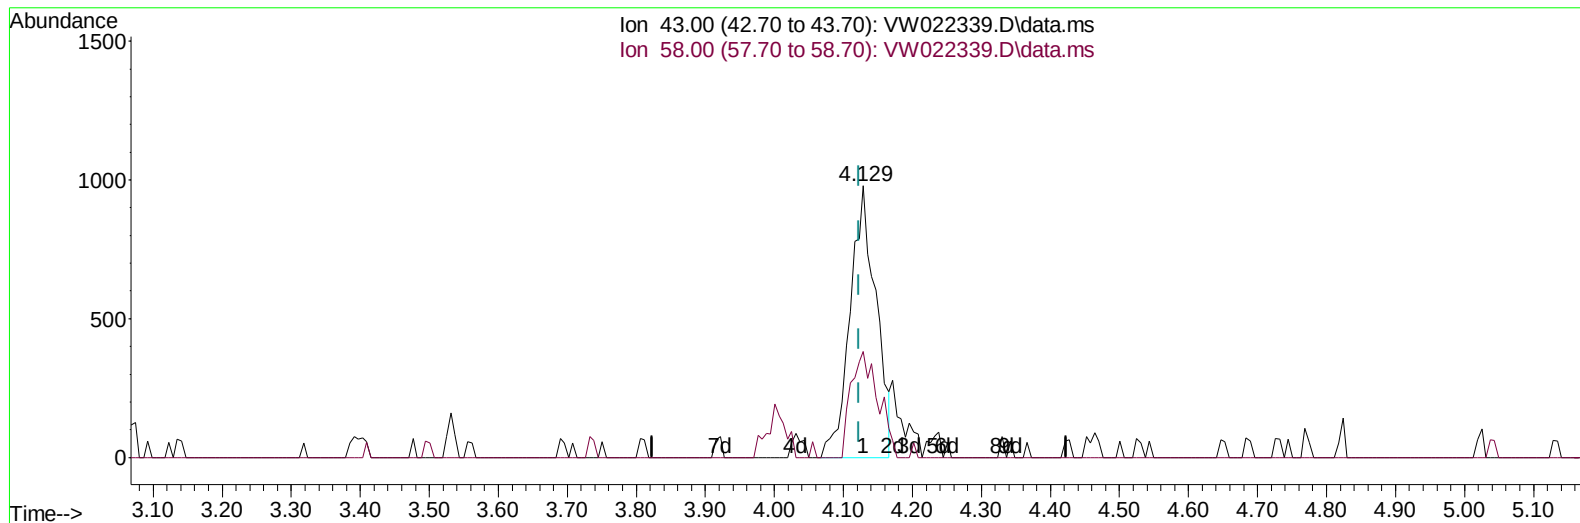

TIC: VW022339.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 8.04 ug/L

response 2548

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	35.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022339.D
 Acq On : 15 Mar 2022 15:59
 Operator : SY/VA
 Sample : N1883-16
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB3

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:35:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

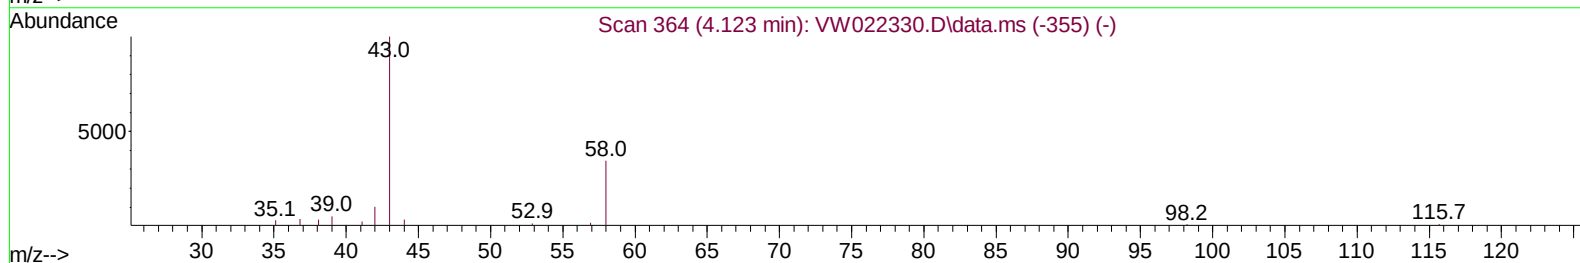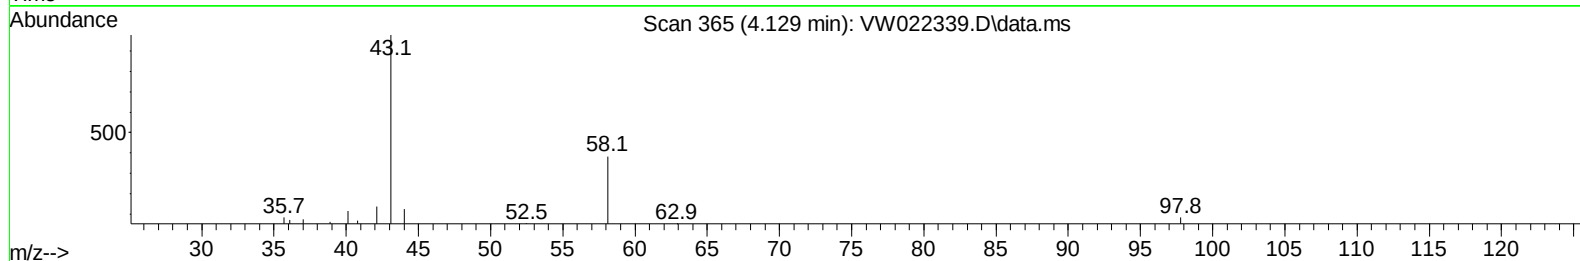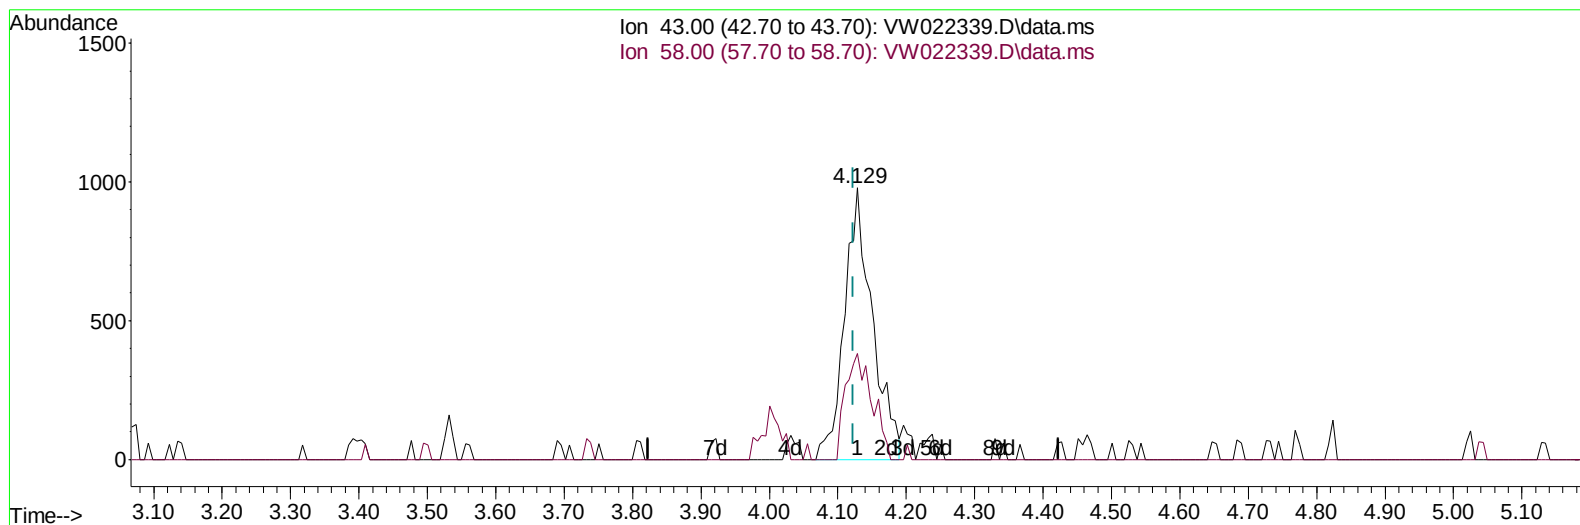

TIC: VW022339.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 8.78 ug/L m

response 2780

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	32.34
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022339.D
 Acq On : 15 Mar 2022 15:59
 Operator : SY/VA
 Sample : N1883-16
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB3

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:35:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	176833	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	166617	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78042	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	45245	19.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.480%	
7) Chloroethane-d5	2.891	69	37222	20.511	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.040%	
11) 1,1-Dichloroethene-d2	4.019	63	49404	13.987	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.960%	
21) 2-Butanone-d5	7.073	46	18561	47.863	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.720%	
24) Chloroform-d	7.646	84	85850	21.760	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	87.040%	
26) 1,2-Dichloroethane-d4	8.305	65	45195	22.037	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	88.160%	
32) Benzene-d6	8.274	84	160076	20.643	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.560%	
36) 1,2-Dichloropropane-d6	9.274	67	47103	21.873	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.480%	
41) Toluene-d8	10.323	98	148817	19.304	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.200%	
43) trans-1,3-Dichloroprop...	10.579	79	18534	19.411	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.640%	
47) 2-Hexanone-d5	10.920	63	14776	41.718	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	83.440%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	42396	22.433	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.720%	
66) 1,2-Dichlorobenzene-d4	13.853	152	57747	23.038	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.160%	
Target Compounds						Qvalue
13) Acetone	4.129	43	2780m	8.777	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022339.D
Acq On : 15 Mar 2022 15:59
Operator : SY/VA
Sample : N1883-16
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:35:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

