




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022340.D
Acq On : 15 Mar 2022 16:23
Operator : SY/VA
Sample : N1883-09
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSA8

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:35:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

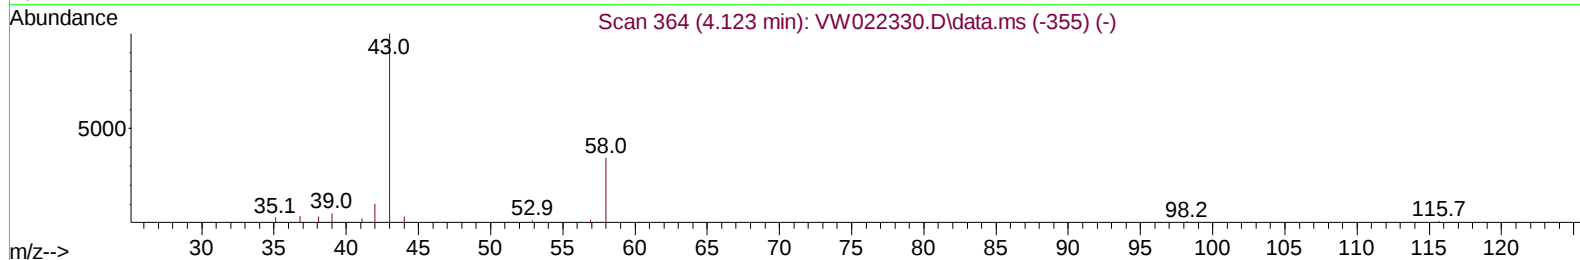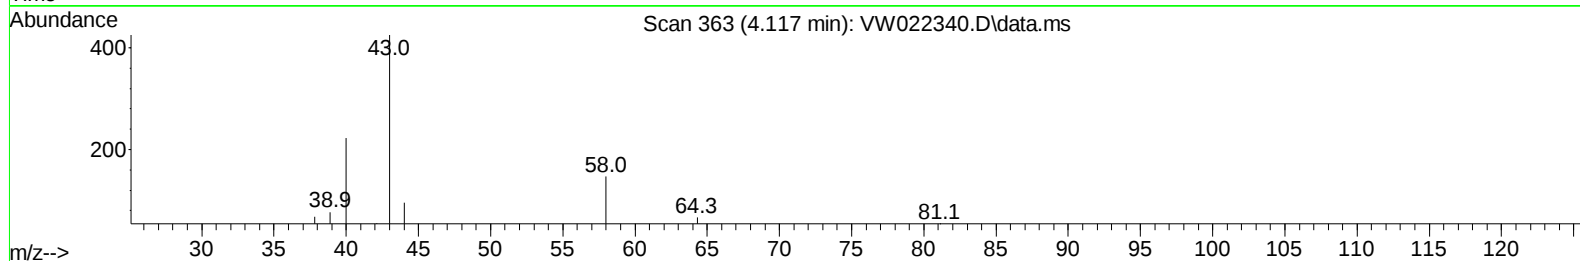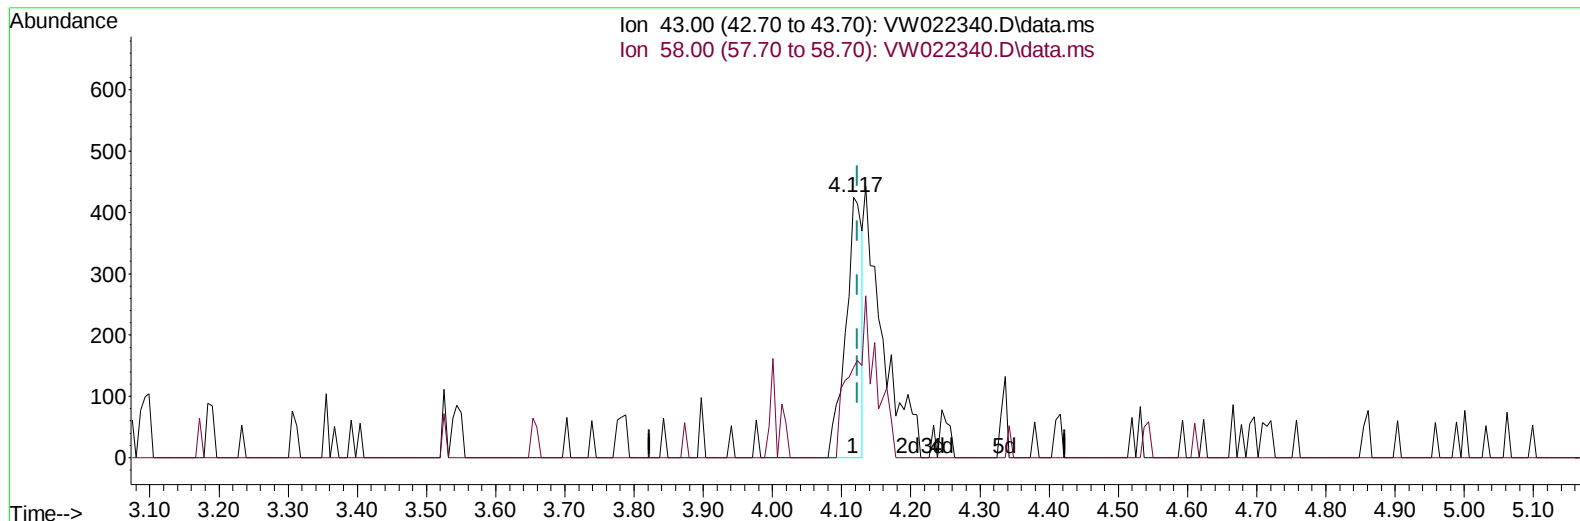

TIC: VW022340.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 2.80 ug/L

response 704

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	6.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022340.D
Acq On : 15 Mar 2022 16:23
Operator : SY/VA
Sample : N1883-09
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSA8

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:35:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

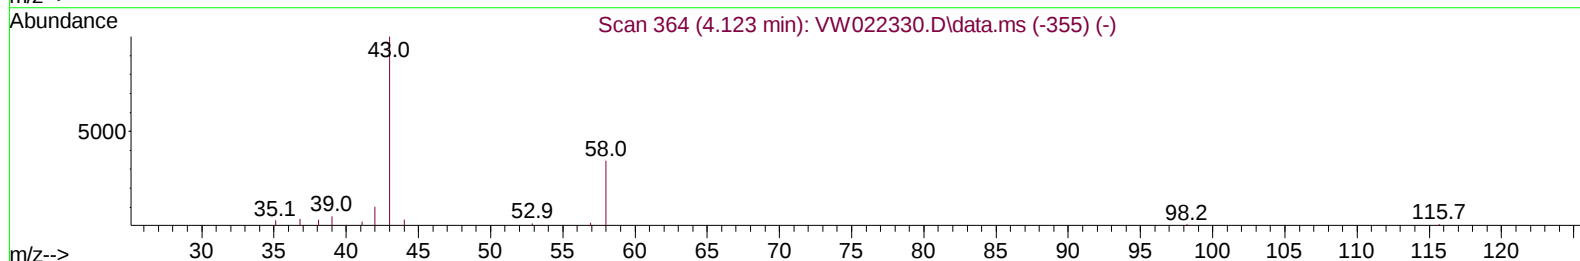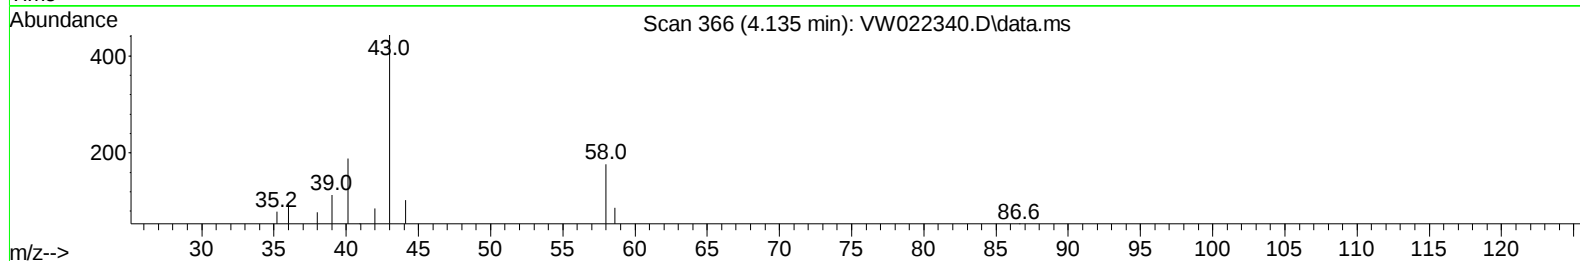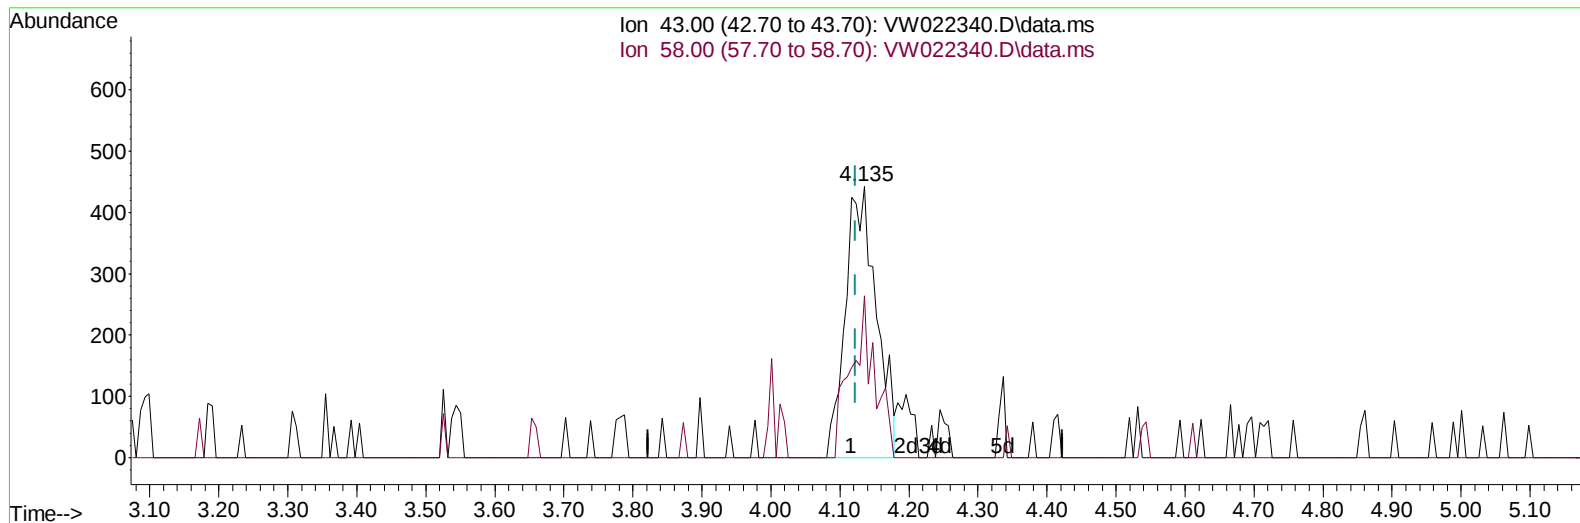

TIC: VW022340.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.47 ug/L m

response 1377

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	3.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022340.D
 Acq On : 15 Mar 2022 16:23
 Operator : SY/VA
 Sample : N1883-09
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:35:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	140460	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	130692	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63412	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	36661	20.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.040%	
7) Chloroethane-d5	2.885	69	28456	19.741	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.960%	
11) 1,1-Dichloroethene-d2	4.013	63	39510	14.083	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.320%	
21) 2-Butanone-d5	7.080	46	17066	55.404	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.800%	
24) Chloroform-d	7.647	84	71633	22.858	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.440%	
26) 1,2-Dichloroethane-d4	8.305	65	38427	23.589	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	94.360%	
32) Benzene-d6	8.275	84	129625	21.311	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	85.240%	
36) 1,2-Dichloropropane-d6	9.275	67	38835	22.991	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.960%	
41) Toluene-d8	10.323	98	120261	19.888	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.560%	
43) trans-1,3-Dichloroprop...	10.579	79	15886	21.211	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.840%	
47) 2-Hexanone-d5	10.927	63	13676	49.227	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	38339	25.862	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	103.440%	
66) 1,2-Dichlorobenzene-d4	13.853	152	49361	24.235	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.960%	
Target Compounds						Qvalue
13) Acetone	4.135	43	1377m	5.473	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022340.D
Acq On : 15 Mar 2022 16:23
Operator : SY/VA
Sample : N1883-09
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSA8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:35:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

