




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022344.D
 Acq On : 15 Mar 2022 17:59
 Operator : SY/VA
 Sample : N1883-13
 Misc : 5.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

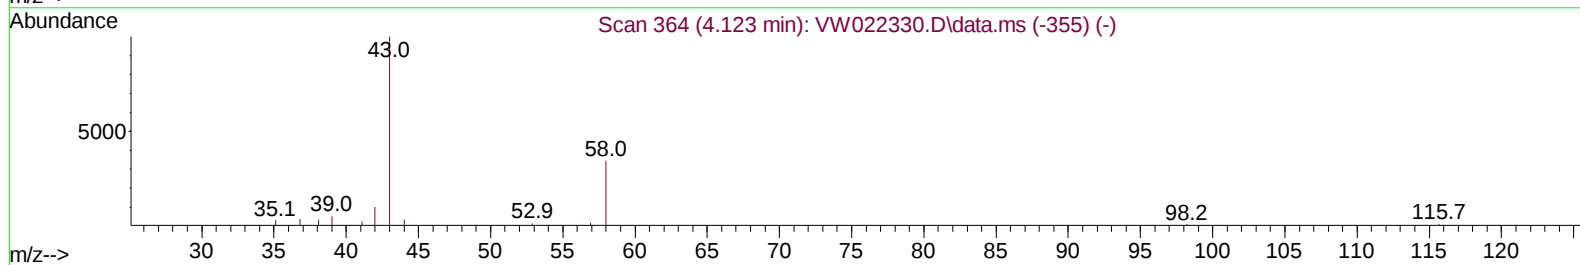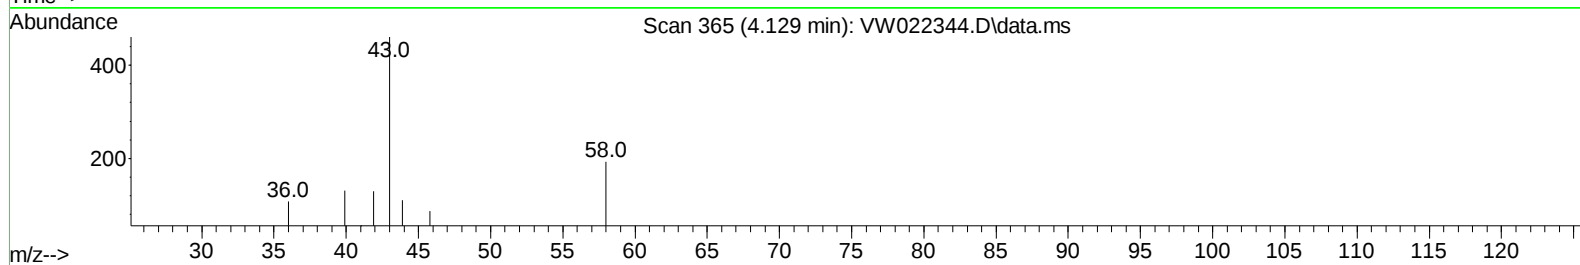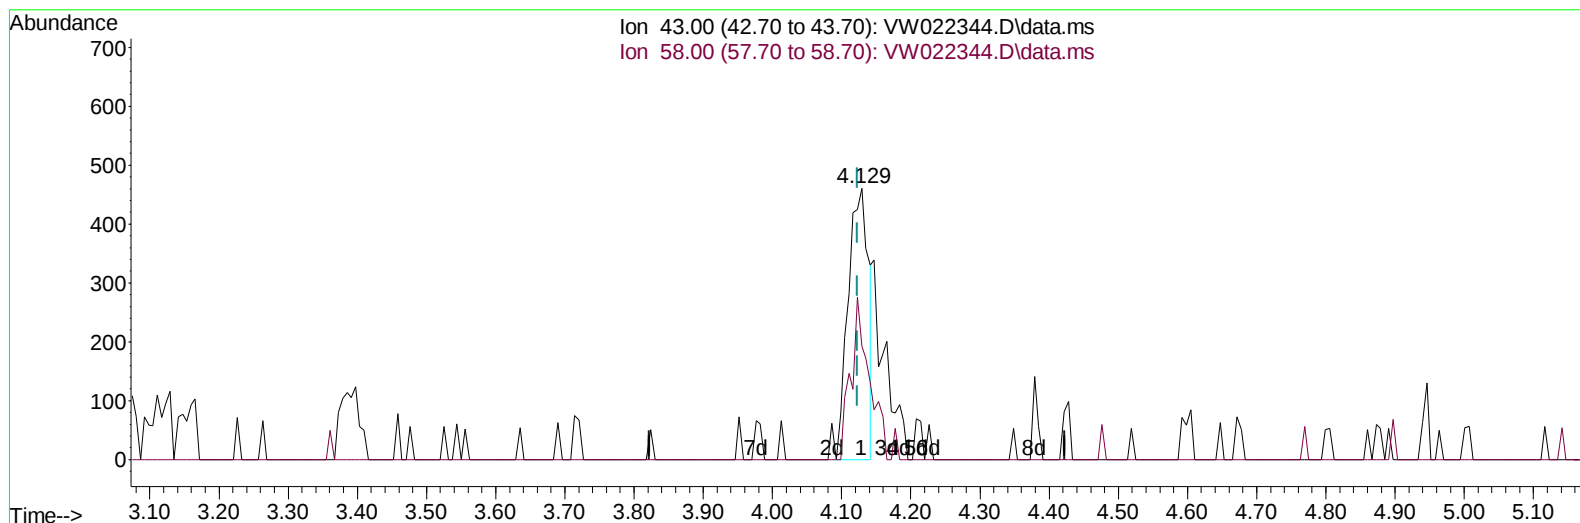

TIC: VW022344.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.05 ug/L

response 937

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	21.99
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022344.D
Acq On : 15 Mar 2022 17:59
Operator : SY/VA
Sample : N1883-13
Misc : 5.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:36:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

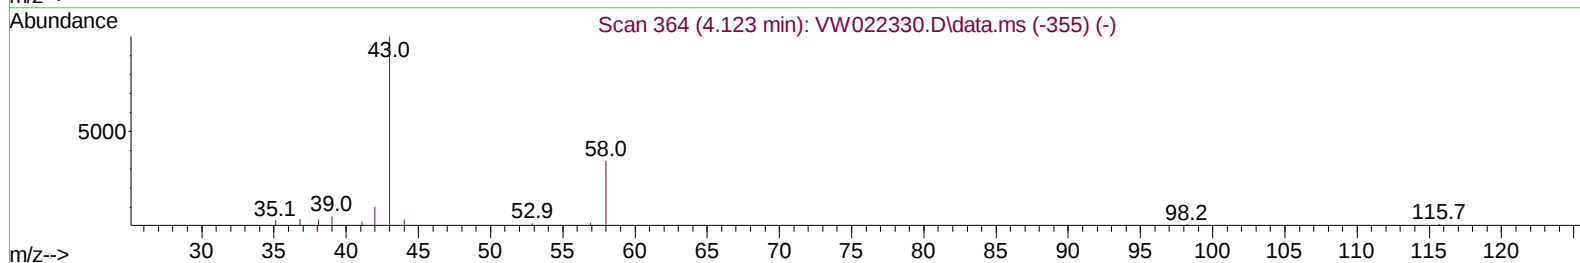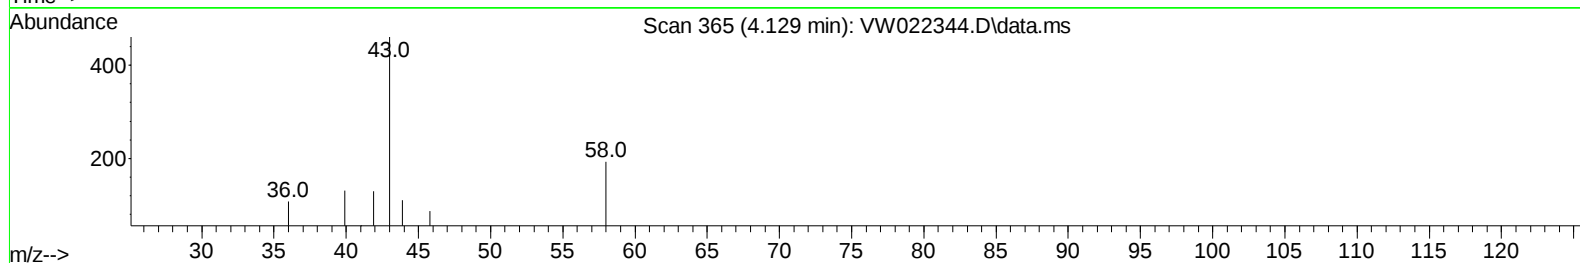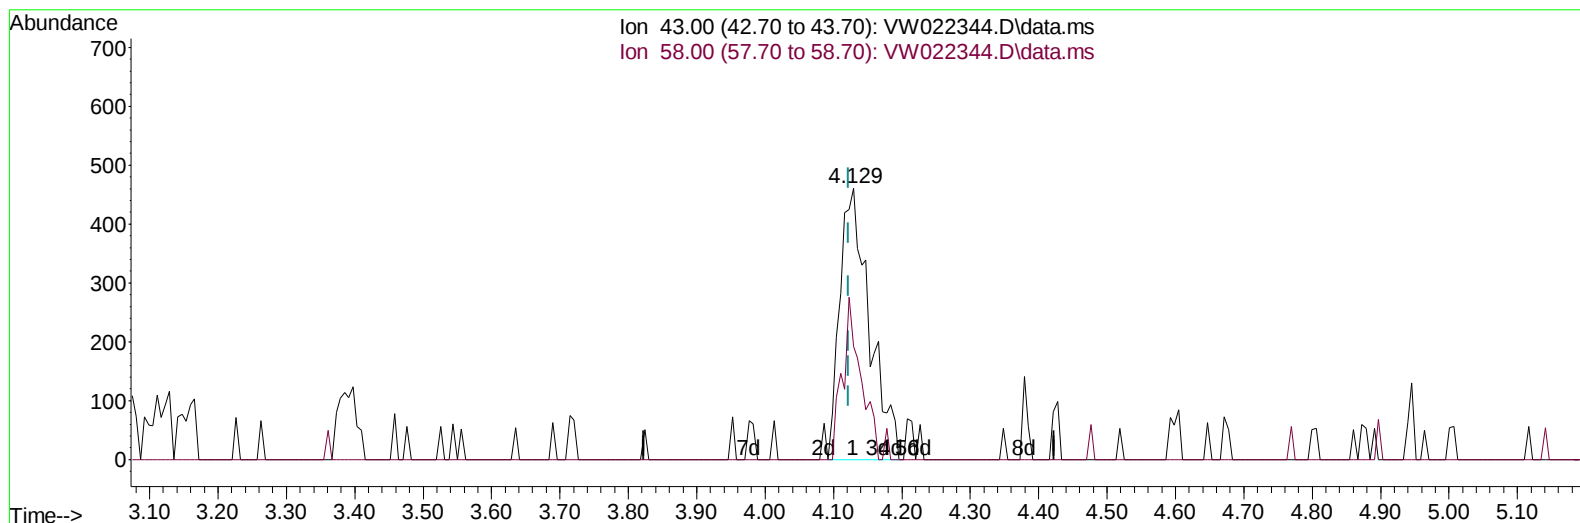

TIC: VW022344.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.94 ug/L m

response 1374

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	14.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022344.D
 Acq On : 15 Mar 2022 17:59
 Operator : SY/VA
 Sample : N1883-13
 Misc : 5.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		129233	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		122560	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		59785	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		33386	19.807	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.240%		
7) Chloroethane-d5	2.885	69		23325	17.587	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	70.360%		
11) 1,1-Dichloroethene-d2	4.019	63		36947	14.313	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.240%		
21) 2-Butanone-d5	7.080	46		23886	84.281	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	168.560%#		
24) Chloroform-d	7.653	84		68586	23.787	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	95.160%		
26) 1,2-Dichloroethane-d4	8.305	65		41411	27.629	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	110.520%		
32) Benzene-d6	8.274	84		124763	21.873	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.480%		
36) 1,2-Dichloropropane-d6	9.274	67		38807	24.499	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	98.000%		
41) Toluene-d8	10.323	98		115008	20.281	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.120%		
43) trans-1,3-Dichloroprop...	10.579	79		17618	25.085	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	100.320%		
47) 2-Hexanone-d5	10.920	63		19167	73.569	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	147.140%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		45450	32.694	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	130.760%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		48449	25.231	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	100.920%		
Target Compounds							
13) Acetone	4.129	43		1374m	5.936	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022344.D
Acq On : 15 Mar 2022 17:59
Operator : SY/VA
Sample : N1883-13
Misc : 5.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:36:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

