




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022345.D
 Acq On : 15 Mar 2022 18:23
 Operator : SY/VA
 Sample : N1883-14
 Misc : 7.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:36:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

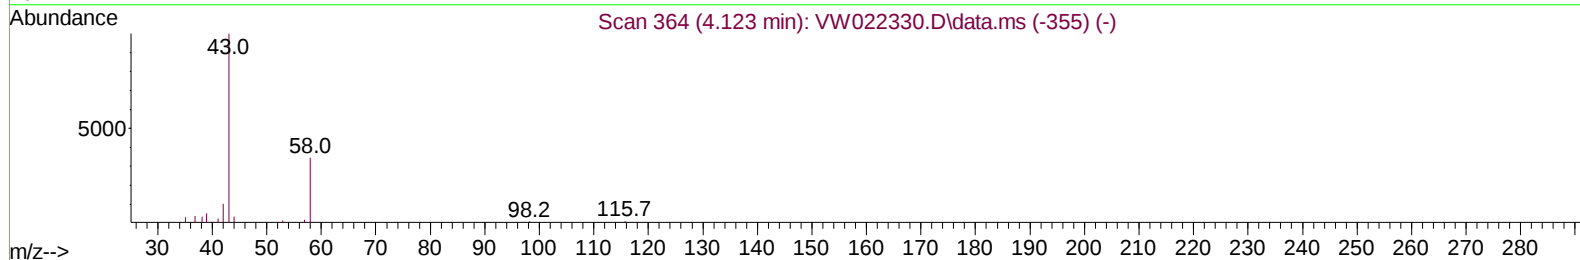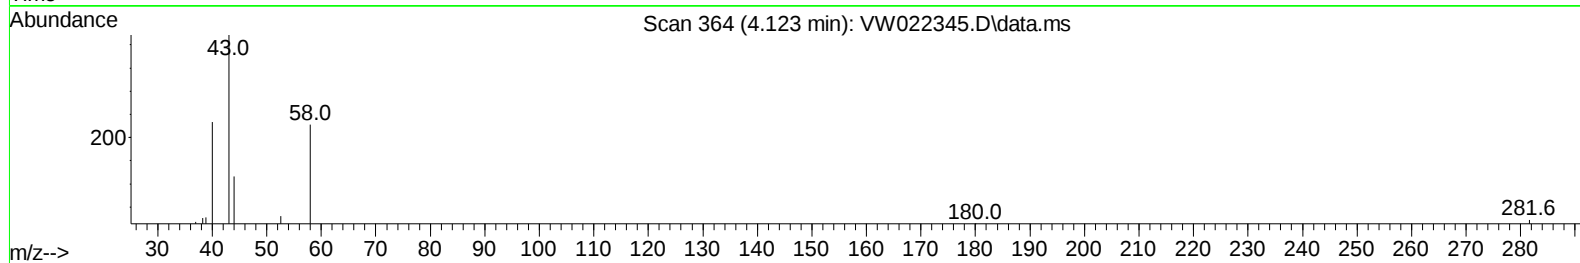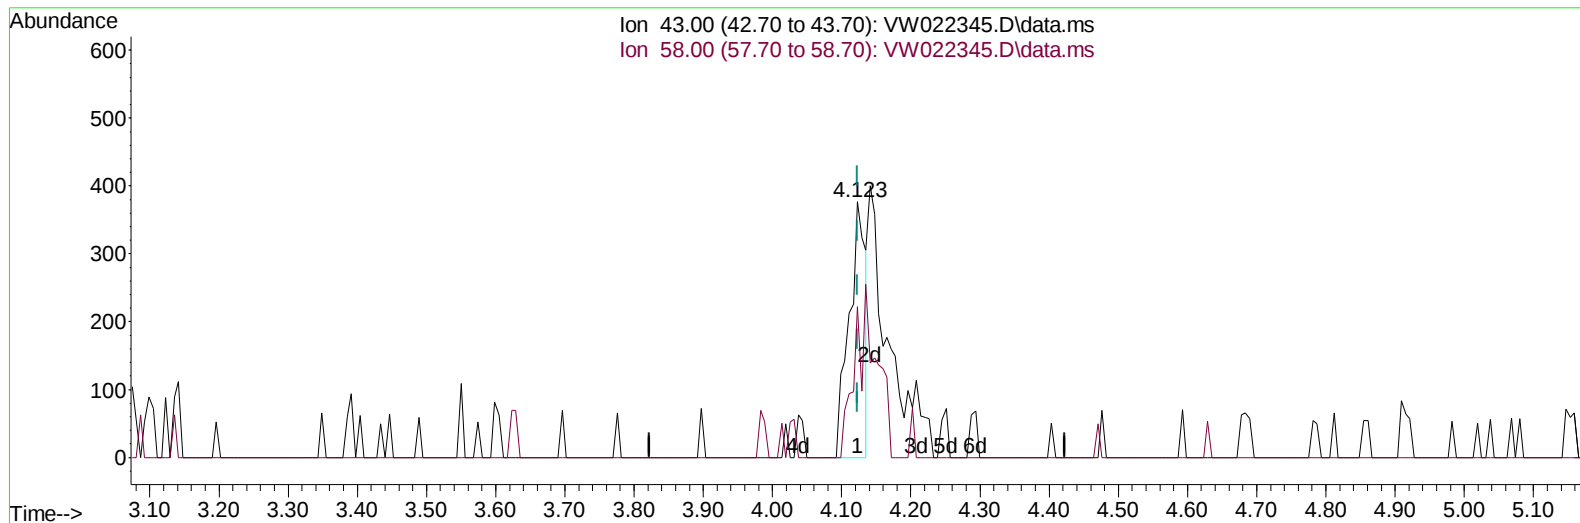

TIC: VW022345.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 2.58 ug/L

response 626

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	33.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022345.D
 Acq On : 15 Mar 2022 18:23
 Operator : SY/VA
 Sample : N1883-14
 Misc : 7.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:36:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

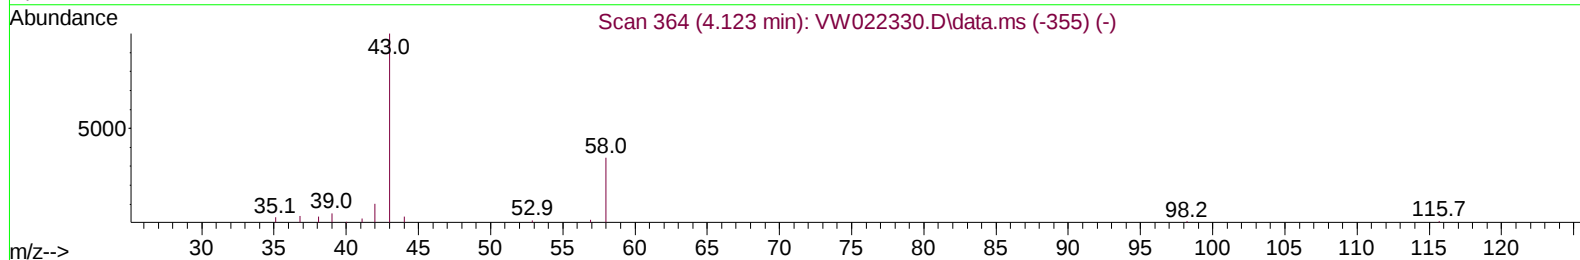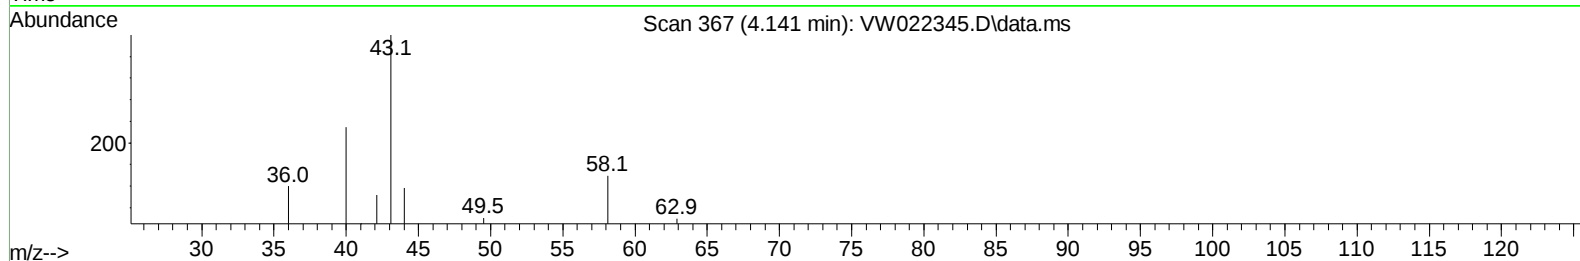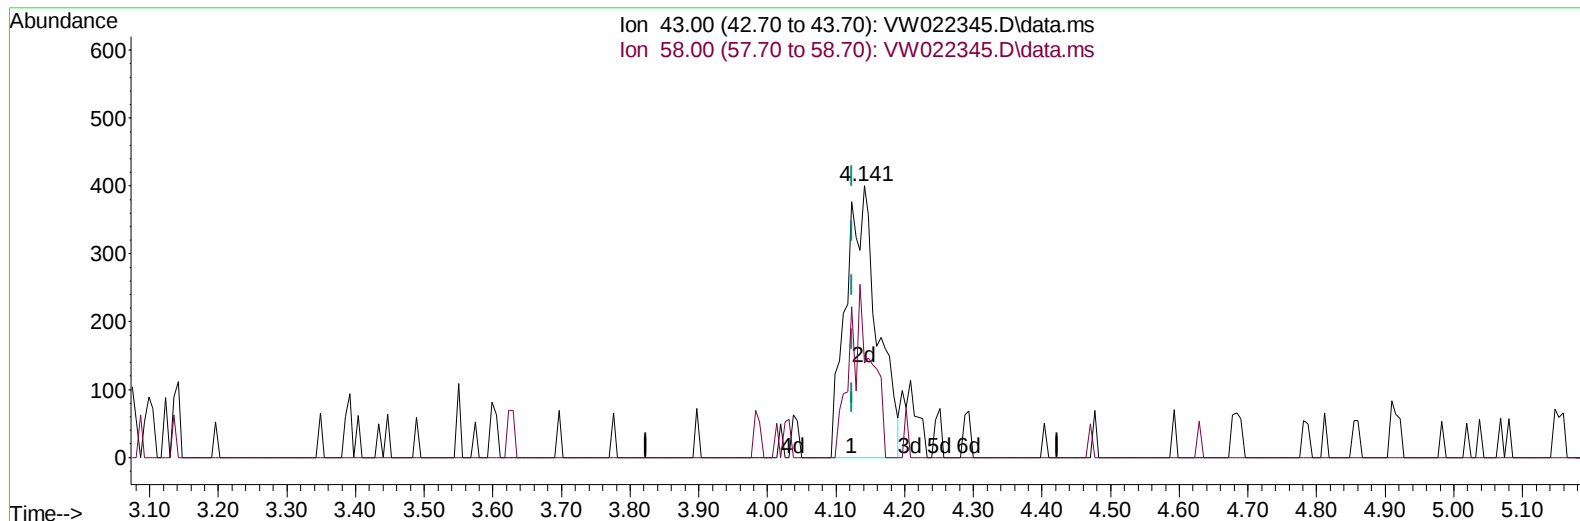

TIC: VW022345.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 5.24 ug/L m

response 1272

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	16.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022345.D
 Acq On : 15 Mar 2022 18:23
 Operator : SY/VA
 Sample : N1883-14
 Misc : 7.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 05:36:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		135620	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		129490	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		62041	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		39027	22.063	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	88.240%		
7) Chloroethane-d5	2.885	69		27711	19.910	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.640%		
11) 1,1-Dichloroethene-d2	4.013	63		40056	14.787	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	59.160%		
21) 2-Butanone-d5	7.074	46		19134	64.334	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	128.660%		
24) Chloroform-d	7.653	84		73184	24.186	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	96.760%		
26) 1,2-Dichloroethane-d4	8.305	65		40669	25.856	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	103.440%		
32) Benzene-d6	8.275	84		132324	21.957	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.840%		
36) 1,2-Dichloropropane-d6	9.274	67		39766	23.761	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	95.040%		
41) Toluene-d8	10.323	98		122554	20.455	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.840%		
43) trans-1,3-Dichloroprop...	10.579	79		16774	22.605	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.400%		
47) 2-Hexanone-d5	10.927	63		15289	55.544	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	111.080%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		40984	27.903	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	111.600%		
66) 1,2-Dichlorobenzene-d4	13.847	152		50783	25.485	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	101.920%		
Target Compounds							
13) Acetone	4.141	43		1272m	5.236	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022345.D
Acq On : 15 Mar 2022 18:23
Operator : SY/VA
Sample : N1883-14
Misc : 7.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:36:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

