

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022340.D
 Acq On : 15 Mar 2022 16:23
 Operator : SY/VA
 Sample : N1883-09
 Misc : 6.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:35:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	140460	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	130692	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63412	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	36661	20.011	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.040%		
7) Chloroethane-d5	2.885	69	28456	19.741	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.960%		
11) 1,1-Dichloroethene-d2	4.013	63	39510	14.083	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.320%		
21) 2-Butanone-d5	7.080	46	17066	55.404	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.800%		
24) Chloroform-d	7.647	84	71633	22.858	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.440%		
26) 1,2-Dichloroethane-d4	8.305	65	38427	23.589	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	94.360%		
32) Benzene-d6	8.275	84	129625	21.311	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.240%		
36) 1,2-Dichloropropane-d6	9.275	67	38835	22.991	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.960%		
41) Toluene-d8	10.323	98	120261	19.888	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	79.560%		
43) trans-1,3-Dichloroprop...	10.579	79	15886	21.211	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.840%		
47) 2-Hexanone-d5	10.927	63	13676	49.227	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.460%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	38339	25.862	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	49361	24.235	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.960%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	1377m	5.473	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022340.D
Acq On : 15 Mar 2022 16:23
Operator : SY/VA
Sample : N1883-09
Misc : 6.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSA8

Quant Time: Mar 16 05:35:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

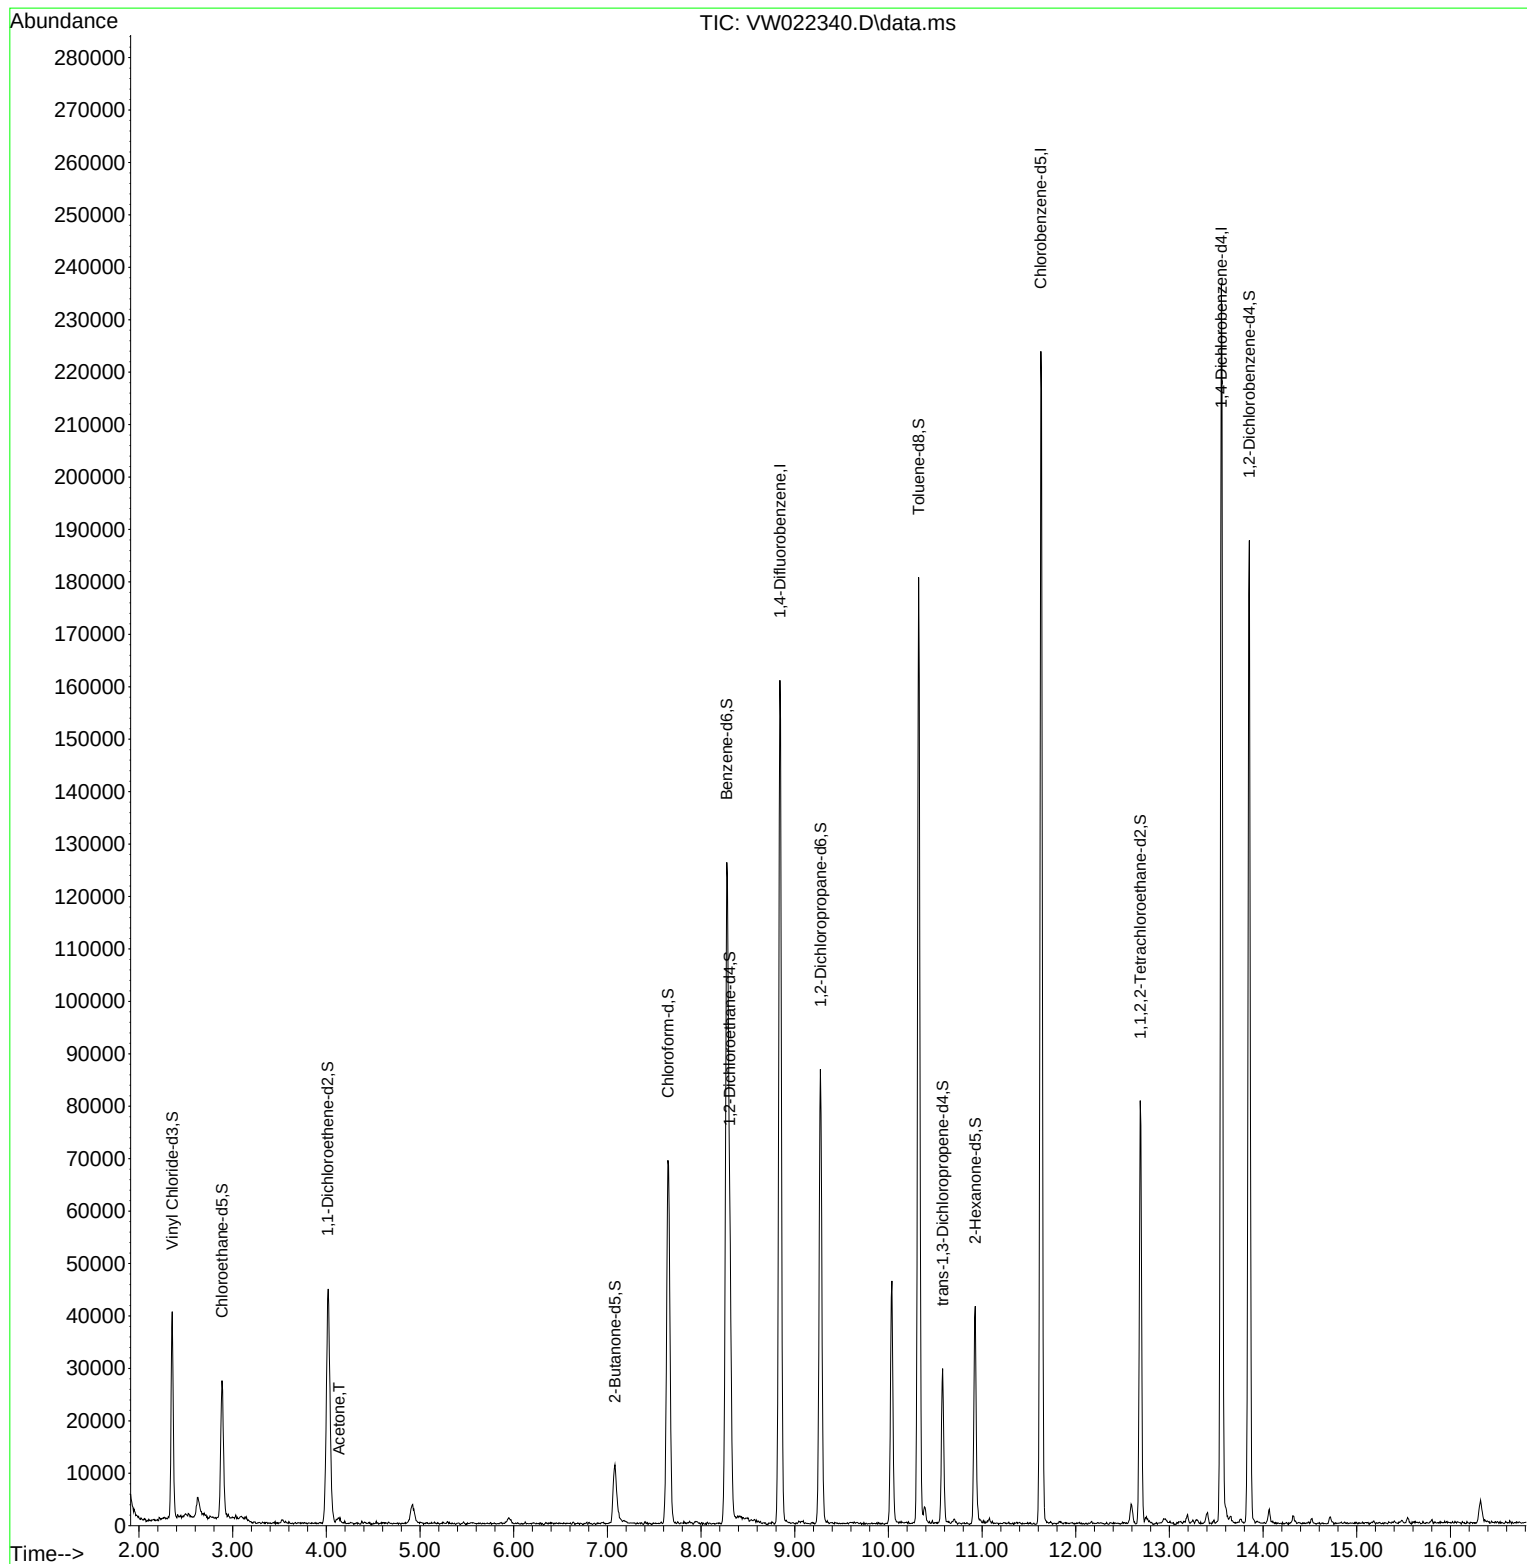

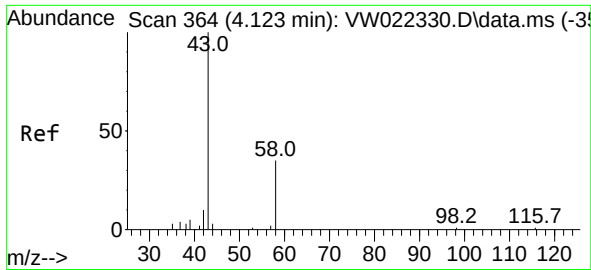

#13

Acetone

Concen: 5.473 ug/L m

RT: 4.135 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW022340.D

Acq: 15 Mar 2022 16:23

Instrument :

MSVOA_W

ClientSampleId :

DBSA8

Tgt Ion: 43 Resp: 137

Ion Ratio Lower Upper

43 100

58 3.1 0.0 69.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022

Supervised By :Mahesh Dadoda 03/16/2022

