

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022344.D
 Acq On : 15 Mar 2022 17:59
 Operator : SY/VA
 Sample : N1883-13
 Misc : 5.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB0

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/16/2022
 Supervised By : Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:36:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	129233	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	122560	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	59785	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	33386	19.807	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.240%		
7) Chloroethane-d5	2.885	69	23325	17.587	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.360%		
11) 1,1-Dichloroethene-d2	4.019	63	36947	14.313	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.240%		
21) 2-Butanone-d5	7.080	46	23886	84.281	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	168.560%#		
24) Chloroform-d	7.653	84	68586	23.787	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.160%		
26) 1,2-Dichloroethane-d4	8.305	65	41411	27.629	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	110.520%		
32) Benzene-d6	8.274	84	124763	21.873	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.480%		
36) 1,2-Dichloropropane-d6	9.274	67	38807	24.499	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.000%		
41) Toluene-d8	10.323	98	115008	20.281	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.120%		
43) trans-1,3-Dichloroprop...	10.579	79	17618	25.085	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	100.320%		
47) 2-Hexanone-d5	10.920	63	19167	73.569	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	147.140%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	45450	32.694	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	130.760%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	48449	25.231	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.920%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	1374m	5.936	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022344.D
Acq On : 15 Mar 2022 17:59
Operator : SY/VA
Sample : N1883-13
Misc : 5.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSB0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022


Quant Time: Mar 16 05:36:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

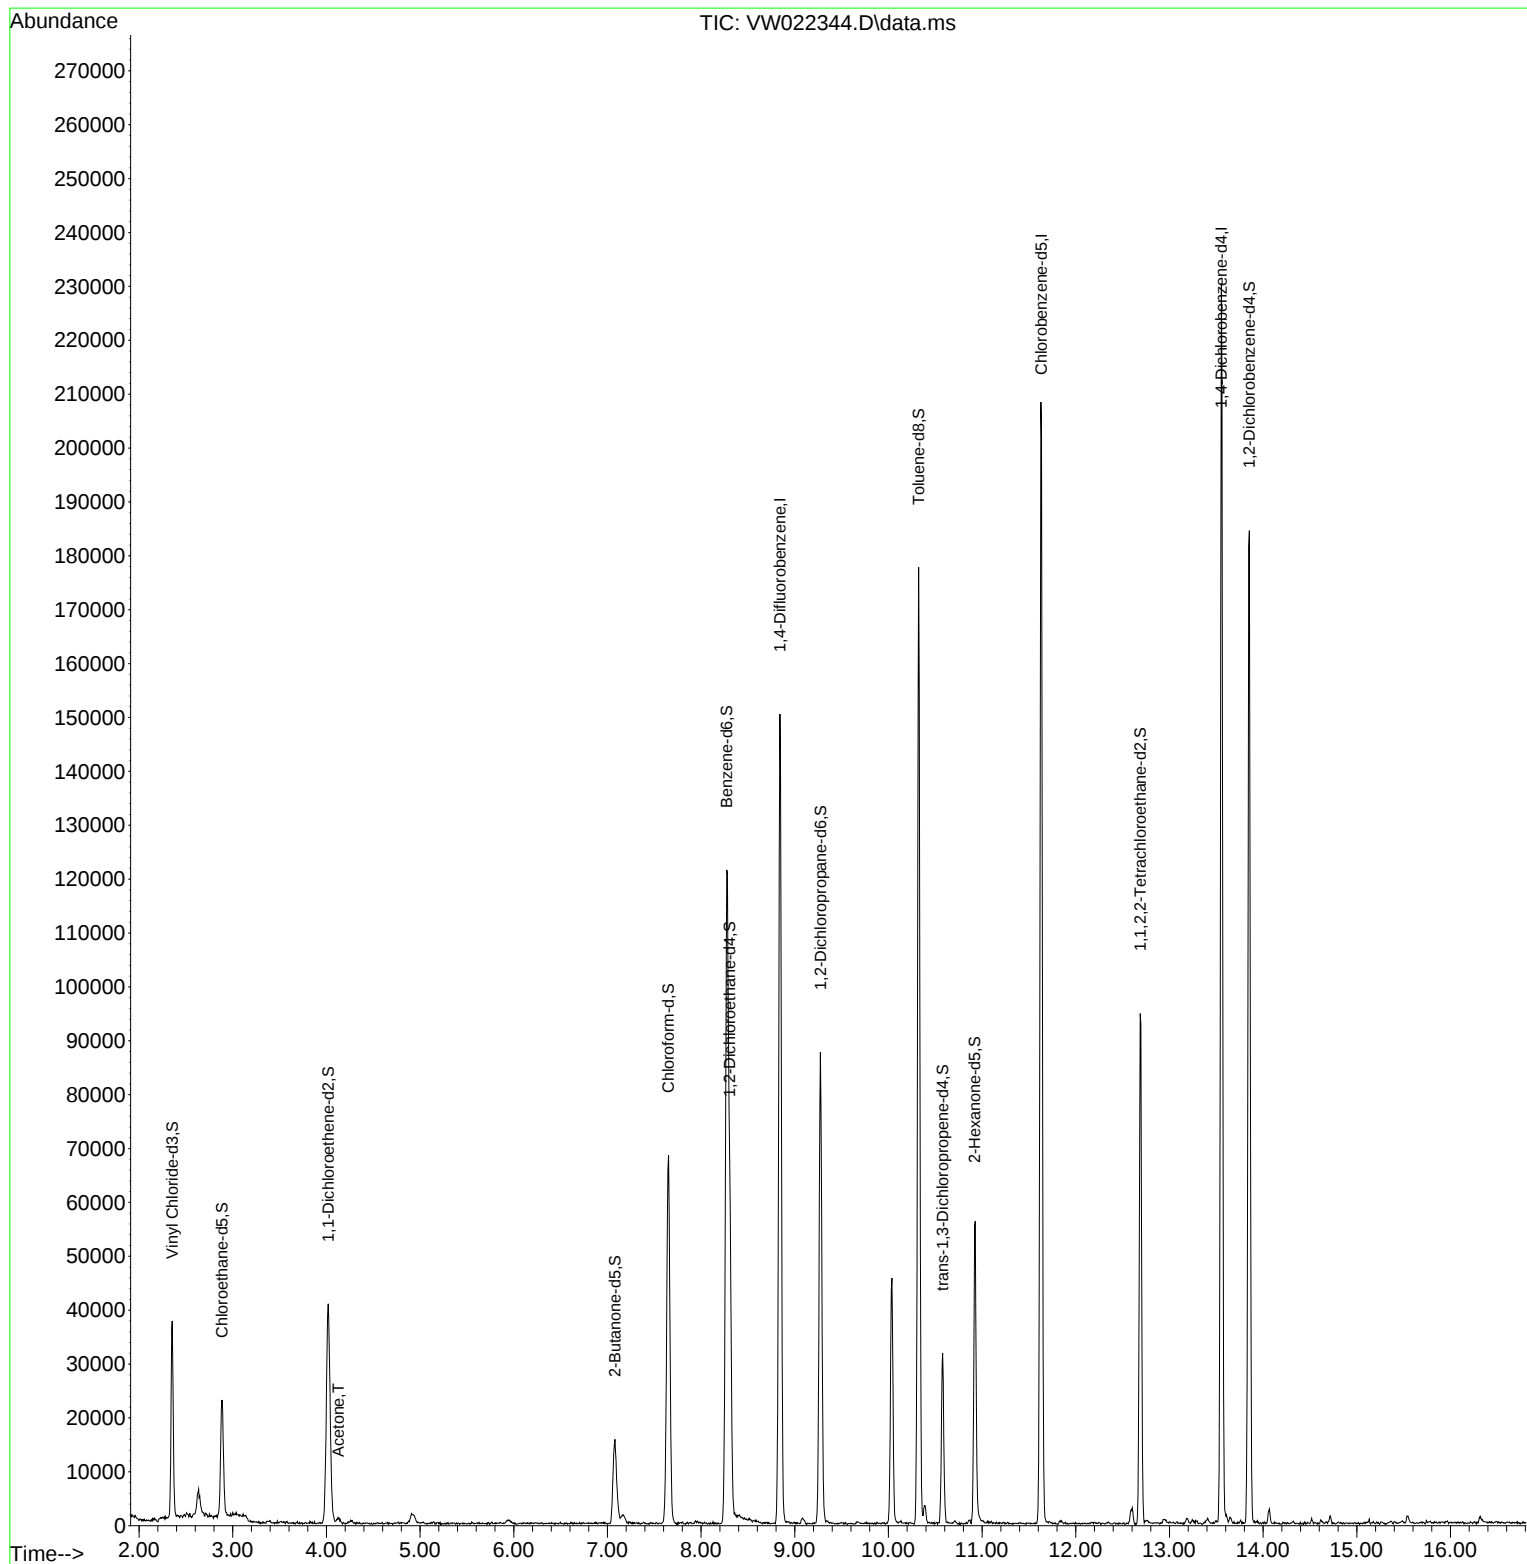

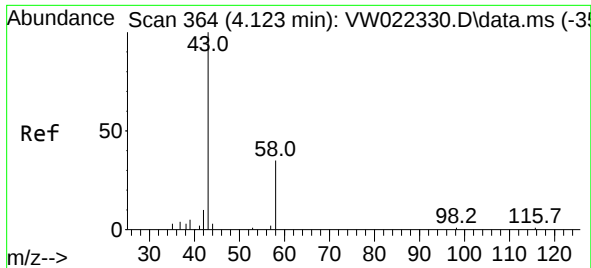

#13
 Acetone
 Concen: 5.936 ug/L m
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022344.D
 Acq: 15 Mar 2022 17:59

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB0

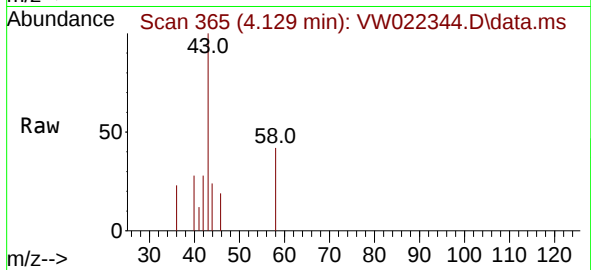

Tgt Ion: 43 Resp: 1374
 Ion Ratio Lower Upper
 43 100
 58 15.0 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

