

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022345.D
 Acq On : 15 Mar 2022 18:23
 Operator : SY/VA
 Sample : N1883-14
 Misc : 7.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:36:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	135620	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	129490	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	62041	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	39027	22.063	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.240%		
7) Chloroethane-d5	2.885	69	27711	19.910	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.640%		
11) 1,1-Dichloroethene-d2	4.013	63	40056	14.787	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.160%		
21) 2-Butanone-d5	7.074	46	19134	64.334	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	128.660%		
24) Chloroform-d	7.653	84	73184	24.186	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.760%		
26) 1,2-Dichloroethane-d4	8.305	65	40669	25.856	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.440%		
32) Benzene-d6	8.275	84	132324	21.957	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.840%		
36) 1,2-Dichloropropane-d6	9.274	67	39766	23.761	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.040%		
41) Toluene-d8	10.323	98	122554	20.455	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.840%		
43) trans-1,3-Dichloroprop...	10.579	79	16774	22.605	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	90.400%		
47) 2-Hexanone-d5	10.927	63	15289	55.544	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.080%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40984	27.903	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	111.600%		
66) 1,2-Dichlorobenzene-d4	13.847	152	50783	25.485	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.920%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	1272m	5.236	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022345.D
Acq On : 15 Mar 2022 18:23
Operator : SY/VA
Sample : N1883-14
Misc : 7.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSB1

Quant Time: Mar 16 05:36:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

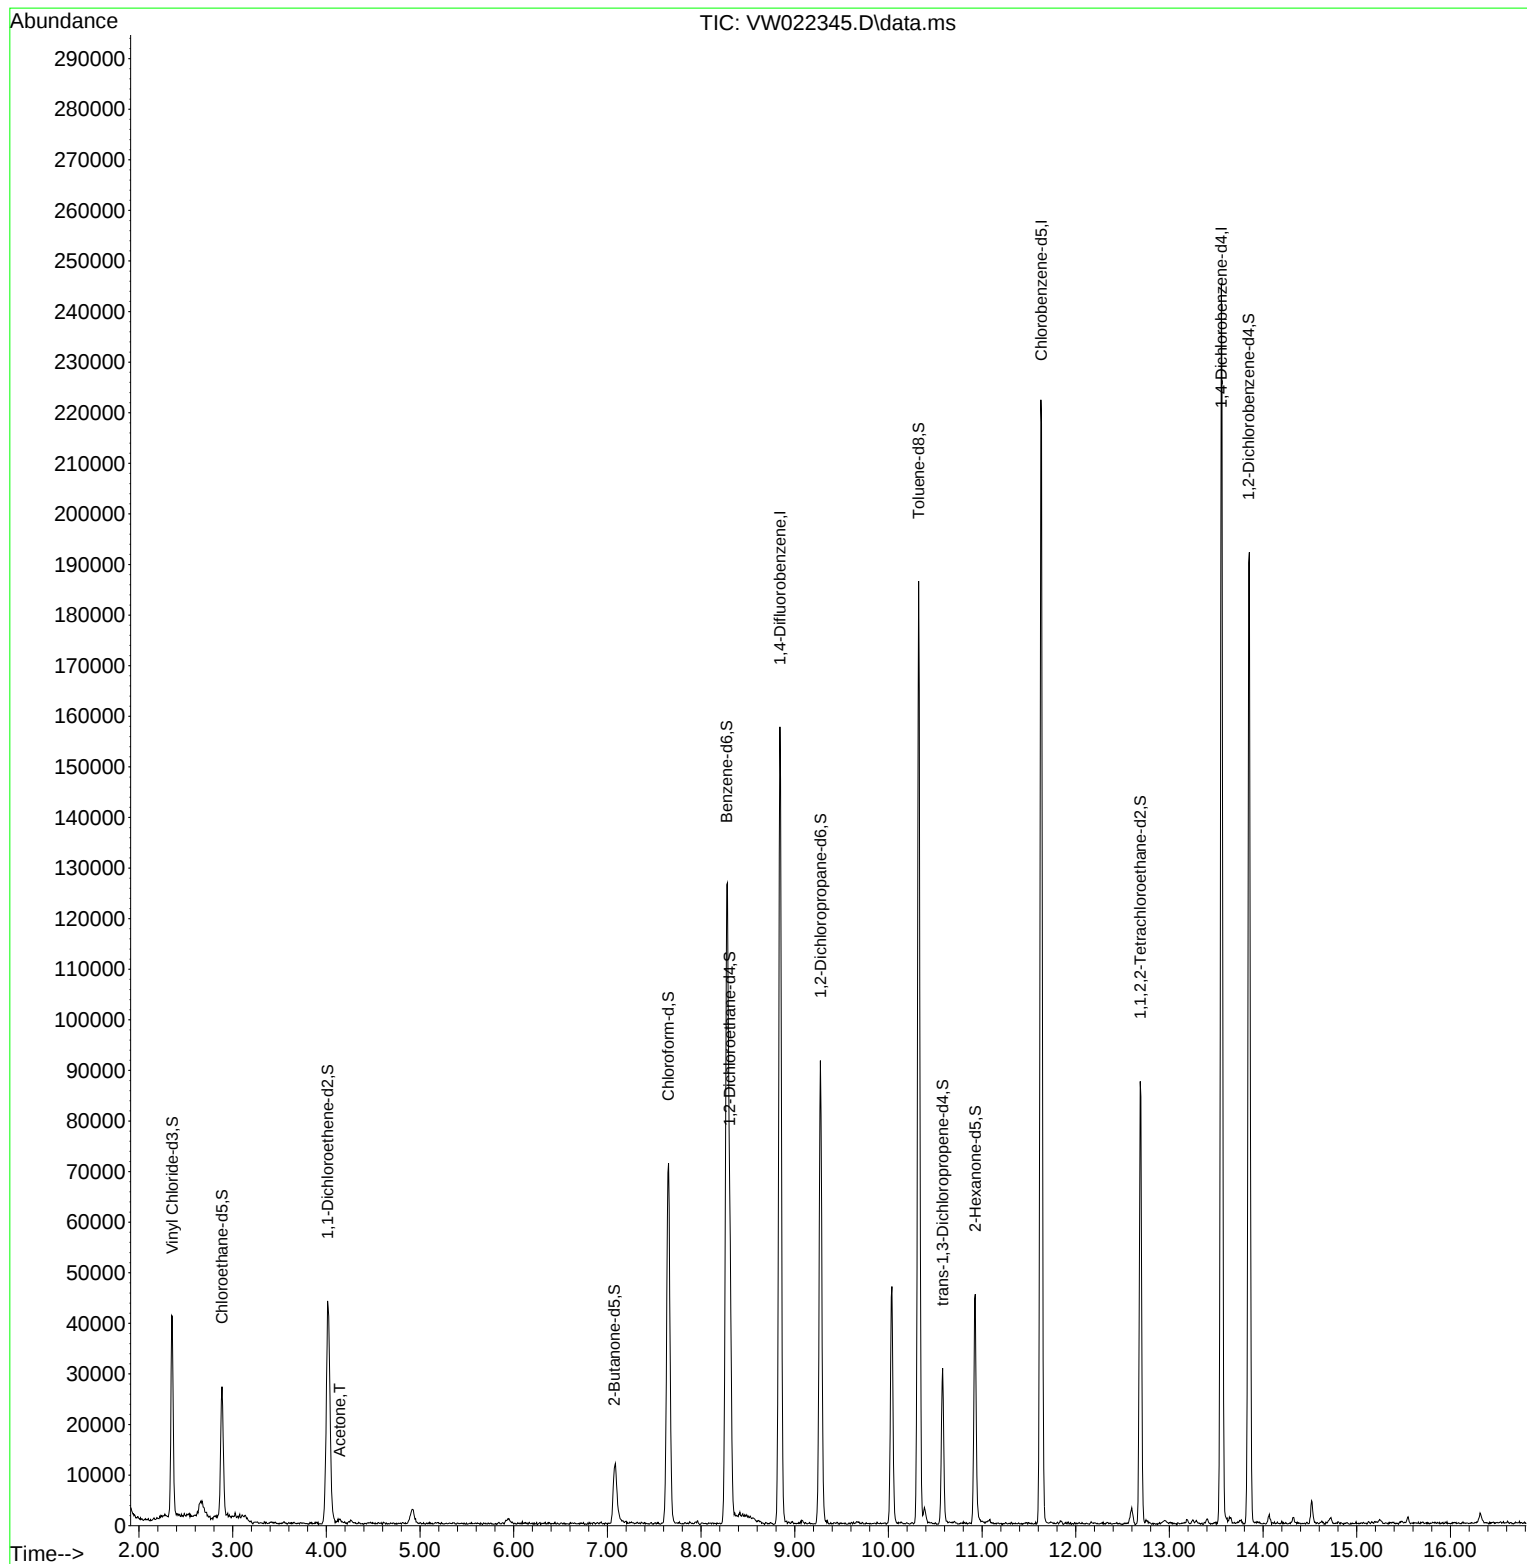

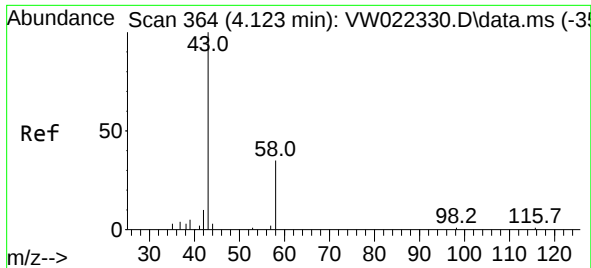

#13
Acetone
Concen: 5.236 ug/L m
RT: 4.141 min Scan# 30
Delta R.T. 0.018 min
Lab File: VW022345.D
Acq: 15 Mar 2022 18:23

Instrument :
MSVOA_W
ClientSampleId :
DBSB1

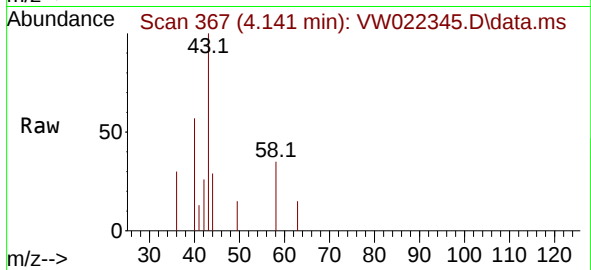

Tgt Ion: 43 Resp: 127
Ion Ratio Lower Upper
43 100
58 16.7 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

