

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022347.D
 Acq On : 15 Mar 2022 19:11
 Operator : SY/VA
 Sample : N1883-06
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 16 05:37:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	94625	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	89842	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	38328	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	28253	22.892	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.560%		
7) Chloroethane-d5	2.885	69	22092	22.750	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.000%		
11) 1,1-Dichloroethene-d2	4.019	63	31399	16.613	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.440%		
21) 2-Butanone-d5	7.080	46	25127	121.086	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	242.180%#		
24) Chloroform-d	7.647	84	53643	25.409	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	101.640%		
26) 1,2-Dichloroethane-d4	8.311	65	30279	27.591	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	110.360%		
32) Benzene-d6	8.275	84	99396	23.772	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.080%		
36) 1,2-Dichloropropane-d6	9.275	67	29939	25.783	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.120%		
41) Toluene-d8	10.323	98	90360	21.737	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.960%		
43) trans-1,3-Dichloroprop...	10.579	79	12646	24.562	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	98.240%		
47) 2-Hexanone-d5	10.921	63	18132	94.942	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	189.880%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	38611	37.889	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	151.560%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	34384	27.930	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	111.720%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	1740m	10.266	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022347.D
Acq On : 15 Mar 2022 19:11
Operator : SY/VA
Sample : N1883-06
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSA5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022


Quant Time: Mar 16 05:37:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

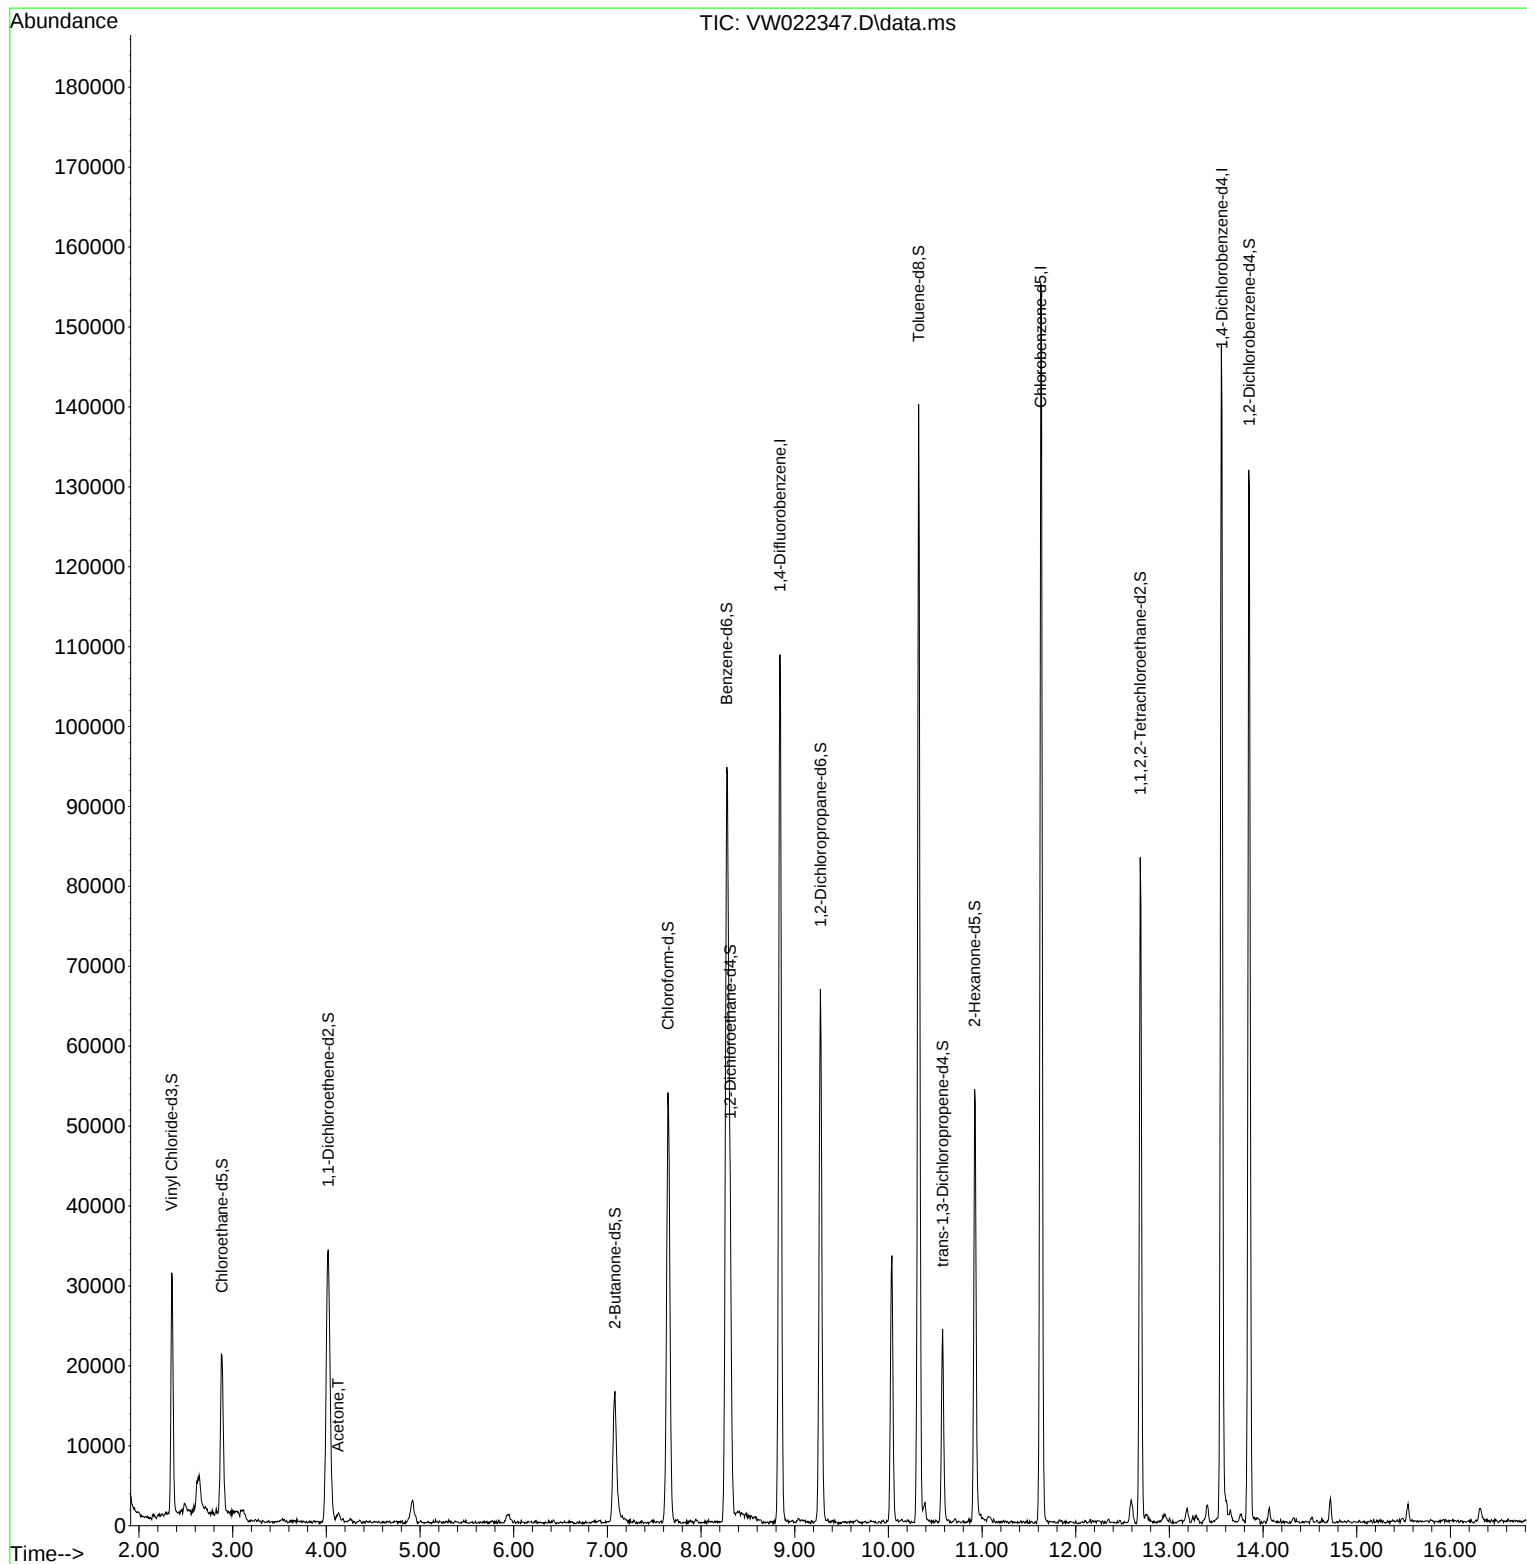

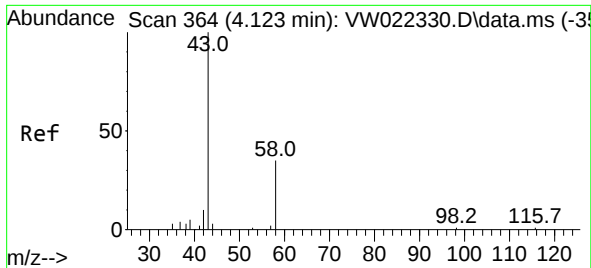

#13
 Acetone
 Concen: 10.266 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW022347.D
 Acq: 15 Mar 2022 19:11

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA5

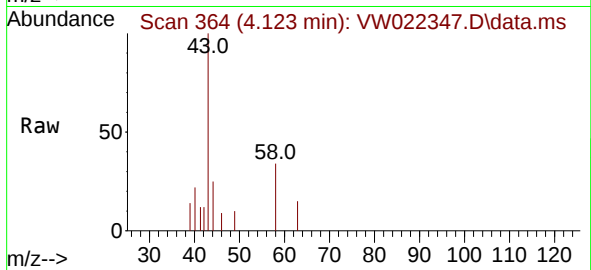

Tgt Ion: 43 Resp: 1740
 Ion Ratio Lower Upper
 43 100
 58 13.0 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

