

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022348.D
 Acq On : 15 Mar 2022 19:35
 Operator : SY/VA
 Sample : N1883-07
 Misc : 5.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA6

Quant Time: Mar 16 05:37:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 16 05:30:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	101309	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	96981	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	45207	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	28043	21.222	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.880%
7) Chloroethane-d5	2.885	69	20215	19.444	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.760%
11) 1,1-Dichloroethene-d2	4.019	63	31320	15.478	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.920%
21) 2-Butanone-d5	7.080	46	19426	87.437	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	174.880%#
24) Chloroform-d	7.647	84	54828	24.256	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.040%
26) 1,2-Dichloroethane-d4	8.305	65	30988	26.374	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.480%
32) Benzene-d6	8.275	84	97693	21.645	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.560%
36) 1,2-Dichloropropane-d6	9.274	67	29586	23.604	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.400%
41) Toluene-d8	10.323	98	89821	20.017	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.080%
43) trans-1,3-Dichloroprop...	10.579	79	11982	21.560	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.240%
47) 2-Hexanone-d5	10.927	63	14634	70.985	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.980%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	34841	31.672	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	126.680%#
66) 1,2-Dichlorobenzene-d4	13.853	152	37240	25.647	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.600%
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	7.177	96	1837	1.475	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
Data File : VW022348.D
Acq On : 15 Mar 2022 19:35
Operator : SY/VA
Sample : N1883-07
Misc : 5.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSA6

Quant Time: Mar 16 05:37:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 16 05:30:16 2022
Response via : Initial Calibration

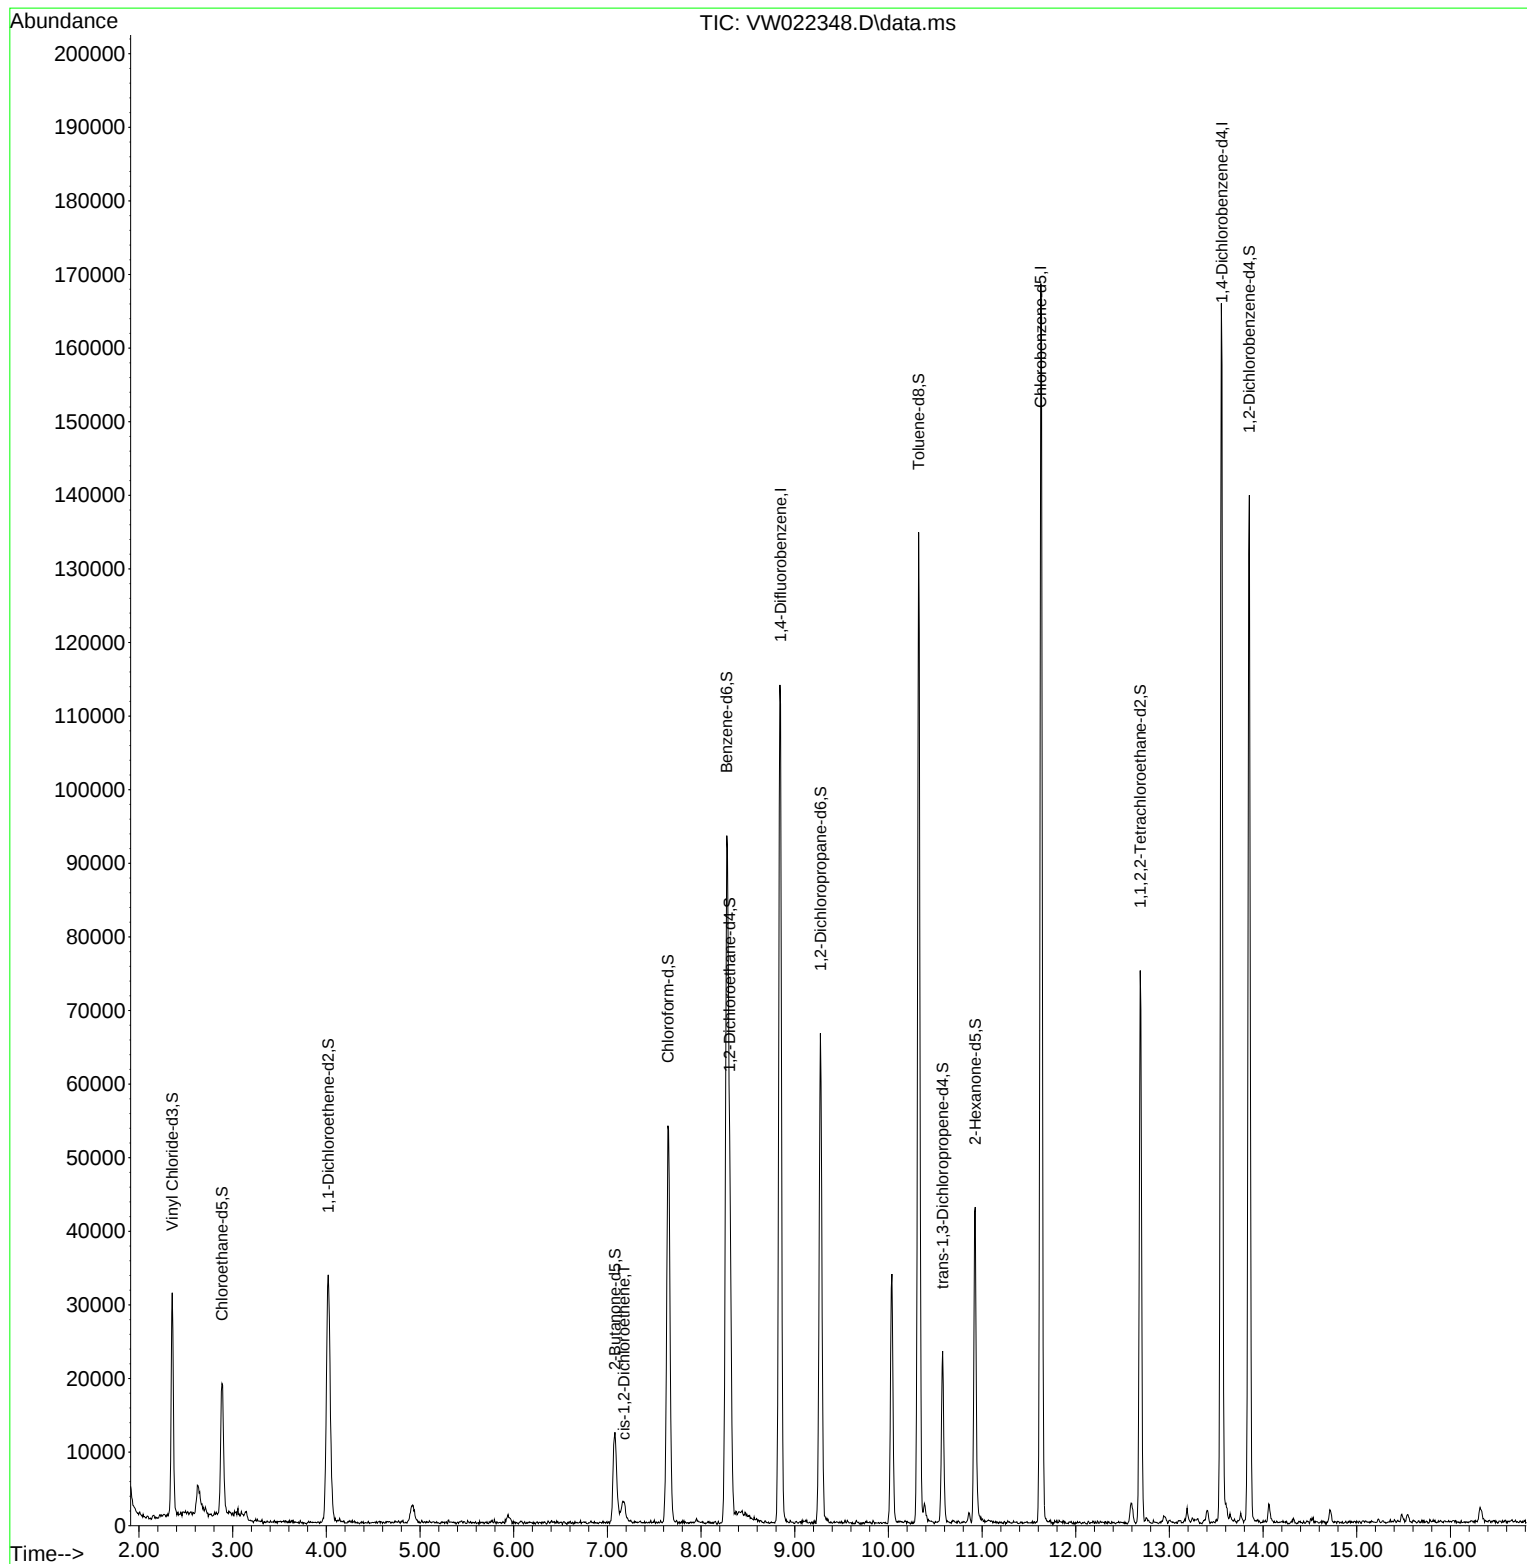

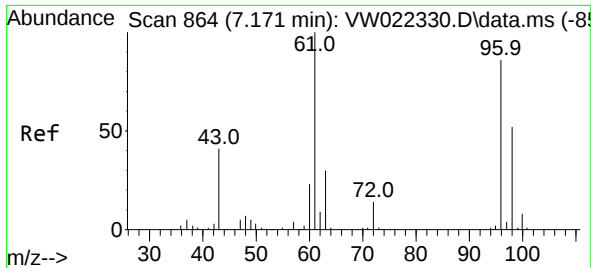

#20
 cis-1,2-Dichloroethene
 Concen: 1.475 ug/L
 RT: 7.177 min Scan# 865
 Delta R.T. 0.006 min
 Lab File: VW022348.D
 Acq: 15 Mar 2022 19:35

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSA6

Tgt Ion: 96 Resp: 1837

Ion	Ratio	Lower	Upper
96	100		
61	103.1	76.8	142.6
68	0.0	0.0	0.0

