
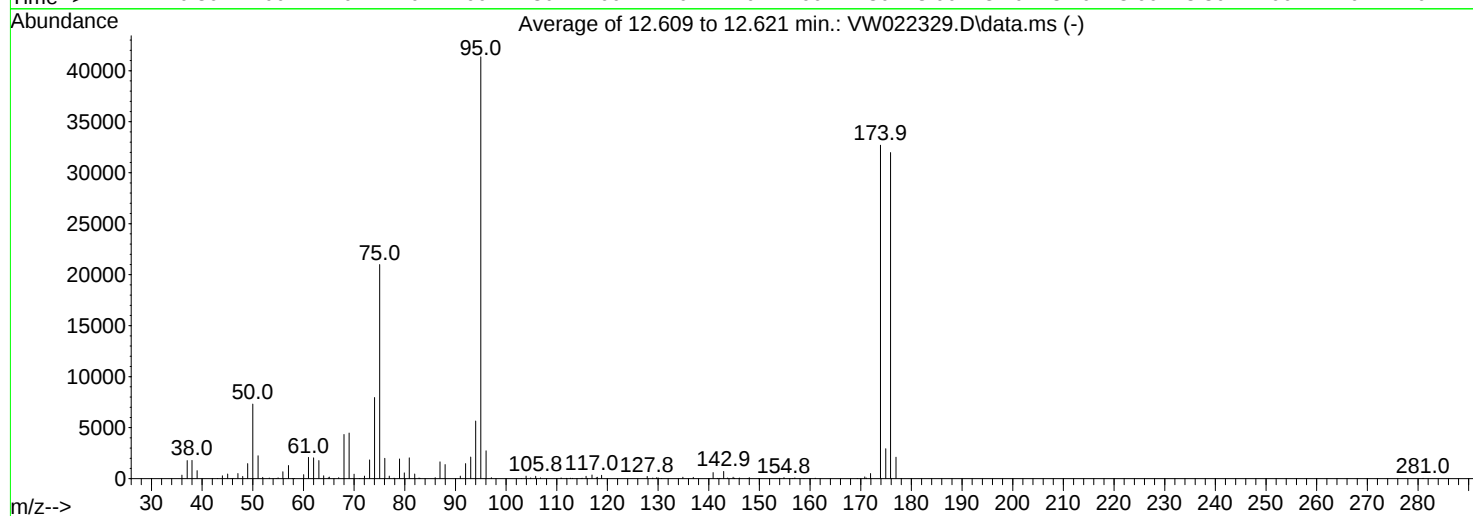


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031522\
 Data File : VW022329.D
 Acq On : 15 Mar 2022 11:09
 Operator : SY/VA
 Sample : BFB523
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB523

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Title : SFAM01.0
 Last Update : Thu Mar 17 00:17:26 2022

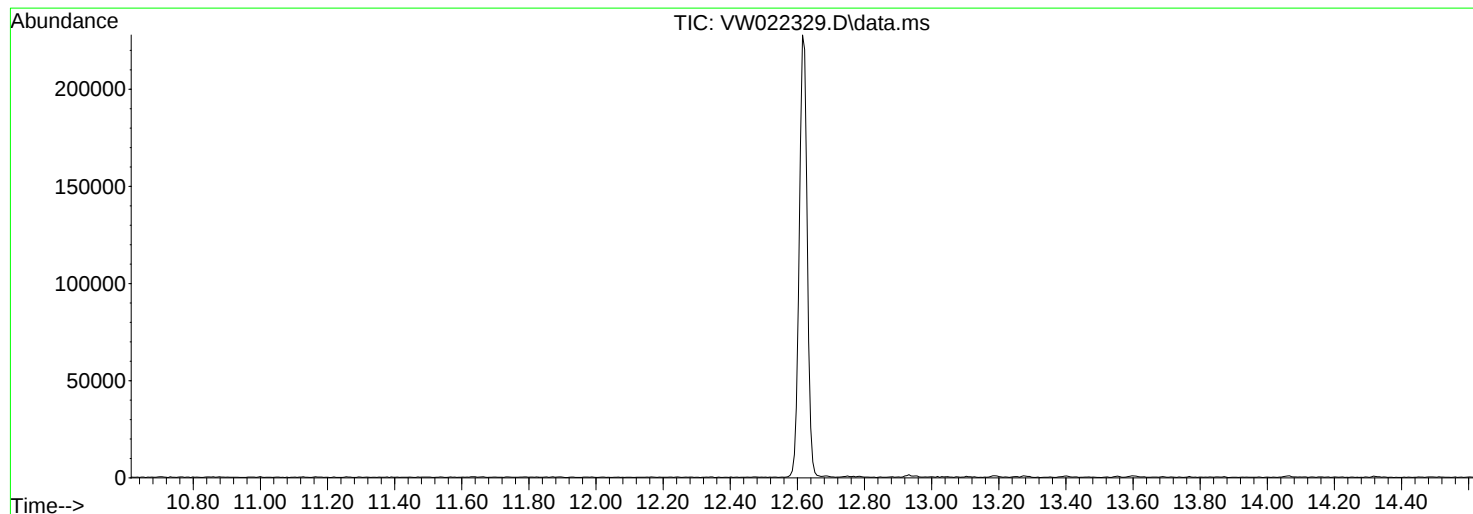

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7306	PASS
75	95	30	80	50.7	20989	PASS
95	95	100	100	100.0	41363	PASS
96	95	5	9	6.6	2726	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.1	32701	PASS
175	174	5	9	9.0	2942	PASS
176	174	95	105	97.8	31984	PASS
177	176	5	10	6.6	2096	PASS

m/z	Abundance
39.90	159.0
40.90	51.0
43.00	61.0
44.00	88.0
50.40	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB523

m/z	Abundance
36.00	274.0
37.10	1482.0
38.00	1603.0
39.00	691.0
40.10	105.0
40.80	62.0
43.10	79.0
44.00	371.0
45.00	366.0
46.10	87.0
47.10	398.0
48.10	137.0
49.00	1464.0
50.00	6814.0
51.10	1962.0
51.90	151.0
53.30	53.0
54.60	54.0
55.10	60.0
56.00	528.0
57.00	1182.0
57.80	54.0
60.00	439.0
61.00	1708.0
62.00	1731.0
63.00	1421.0
64.00	298.0
64.90	221.0
66.90	132.0
68.00	3426.0
69.00	4105.0
70.00	316.0
72.00	217.0
73.00	1753.0
74.00	7031.0
75.00	17736.0
76.10	1688.0
76.90	240.0
78.90	1771.0
79.90	534.0
80.90	1867.0
82.00	383.0
82.80	88.0
86.00	108.0
87.00	1508.0
88.00	1217.0
90.90	161.0
92.00	1194.0
93.00	1828.0
94.00	4949.0
95.00	34904.0
96.00	2383.0
97.10	121.0
103.90	200.0
104.80	67.0
105.90	194.0
106.70	74.0
110.90	75.0
111.90	99.0
113.10	94.0
114.80	68.0
115.70	109.0
116.00	108.0
116.90	326.0
117.80	230.0
118.90	254.0
127.90	228.0
129.70	173.0
134.90	131.0
136.90	136.0
140.00	61.0
141.00	439.0
141.70	80.0
142.90	647.0
143.70	67.0
144.90	147.0
147.70	56.0
149.90	54.0
154.80	85.0
156.90	81.0
158.80	62.0
170.90	144.0
171.90	415.0
173.90	24960.0
175.00	2264.0
175.90	24648.0
176.90	1623.0

Instrument :
MSVOA_W
ClientSampleId :
BFB523

m/z	Abundance
36.00	422.0
37.10	2238.0
38.00	1953.0
39.00	915.0
39.90	209.0
43.20	62.0
44.00	408.0
45.00	581.0
45.70	61.0
47.00	506.0
47.90	246.0
49.00	1708.0
50.00	8315.0
51.00	2426.0
52.00	116.0
53.30	65.0
55.10	67.0
55.90	755.0
57.10	1455.0
60.00	416.0
61.00	2432.0
62.00	2420.0
63.10	2083.0
64.00	334.0
65.10	204.0
68.00	5069.0
69.00	4942.0
70.00	547.0
72.10	330.0
73.00	1858.0
74.00	8421.0
75.00	24224.0
76.10	2226.0
77.00	216.0
79.00	2149.0
79.90	600.0
80.90	2333.0
81.90	534.0
82.80	97.0
86.10	103.0
86.90	1836.0
87.90	1451.0
91.00	269.0
92.00	1735.0
93.00	2408.0
94.00	5927.0
95.00	45736.0
96.10	2954.0
97.10	91.0
103.00	51.0
103.90	274.0
104.90	92.0
105.80	252.0
106.80	99.0
110.80	120.0
112.70	71.0
115.00	131.0
115.80	332.0
117.00	383.0
118.00	176.0
118.70	290.0
127.80	202.0
128.90	58.0
130.00	224.0
134.90	191.0
137.00	93.0
140.80	763.0
142.20	111.0
142.90	887.0
143.80	74.0
144.70	159.0
145.10	146.0
146.00	99.0
148.10	118.0
154.00	97.0
154.90	130.0
157.00	87.0
170.70	126.0
171.10	179.0
171.90	626.0
173.90	33616.0
174.90	3102.0
175.90	35704.0
177.00	2305.0
281.00	96.0

Instrument :
MSVOA_W
ClientSampleId :
BFB523

m/z	Abundance
36.00	329.0
37.00	1583.0
38.00	1818.0
39.00	731.0
40.00	127.0
40.80	69.0
42.00	61.0
43.10	83.0
44.00	339.0
45.10	419.0
47.10	585.0
48.10	295.0
49.00	1267.0
50.00	6788.0
51.00	2332.0
51.90	120.0
53.10	58.0
54.90	118.0
56.00	727.0
57.00	1215.0
58.20	54.0
60.10	321.0
61.00	2116.0
62.00	1953.0
63.00	1822.0
64.00	219.0
65.10	249.0
67.00	138.0
68.00	4490.0
69.00	4367.0
70.00	439.0
71.10	60.0
72.10	230.0
73.10	1914.0
74.10	8404.0
75.10	21008.0
76.00	2051.0
77.00	308.0
77.90	152.0
78.90	1882.0
79.90	551.0
80.90	1946.0
81.90	433.0
83.00	98.0
85.90	62.0
87.00	1581.0
88.00	1459.0
90.90	305.0
92.00	1500.0
93.00	2126.0
94.00	6065.0
95.00	43448.0
96.00	2840.0
97.10	60.0
104.00	295.0
104.80	89.0
105.90	260.0
106.90	55.0
110.80	66.0
112.70	80.0
115.80	268.0
116.90	365.0
118.00	272.0
118.90	449.0
127.90	227.0
129.00	109.0
129.70	115.0
130.70	67.0
134.80	102.0
137.00	142.0
140.80	573.0
143.00	603.0
143.70	69.0
144.80	133.0
146.10	75.0
147.90	173.0
154.90	102.0
156.60	57.0
157.10	83.0
161.00	119.0
169.30	61.0
170.80	228.0
172.00	487.0
173.90	39528.0
175.00	3460.0
175.90	35600.0
177.00	2361.0
178.00	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB523