

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW031619\
Quantitation Report (QT/LSC Reviewed)


Data File : VW009204.D
Acq On : 16 Mar 2019 12:15
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK03

Manual Integrations
APPROVED

MMDadoda
3/19/2019 10:03:15 AM

Quant Time: Mar 18 02:47:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 02:40:38 2019
Response via : Initial Calibration

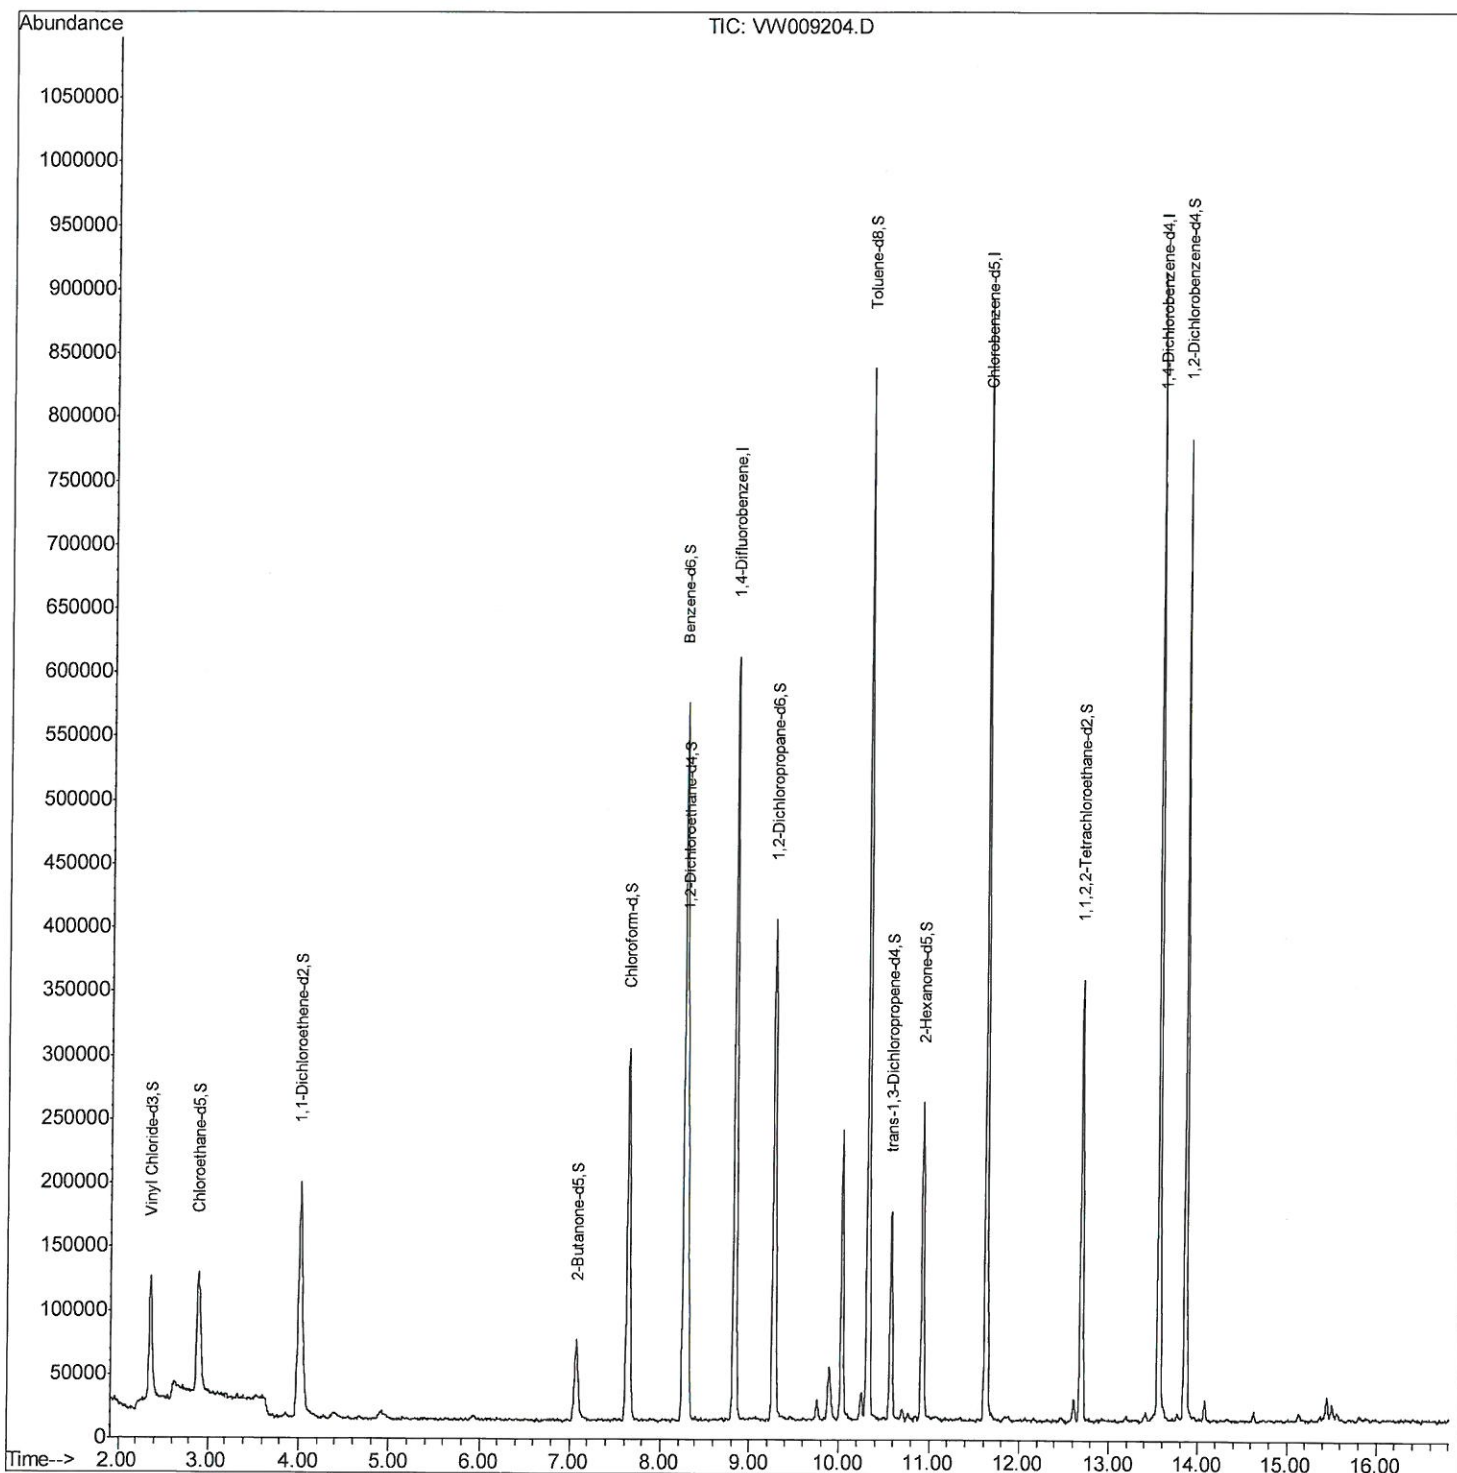

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW031619\
Quantitation Report (Qedit)




Data File : VW009204.D
Acq On : 16 Mar 2019 12:15
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK03

Manual Integrations
APPROVED

MMDadoda
3/19/2019 10:03:15 AM

Quant Time: Mar 18 02:43:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 02:40:38 2019
Response via : Initial Calibration

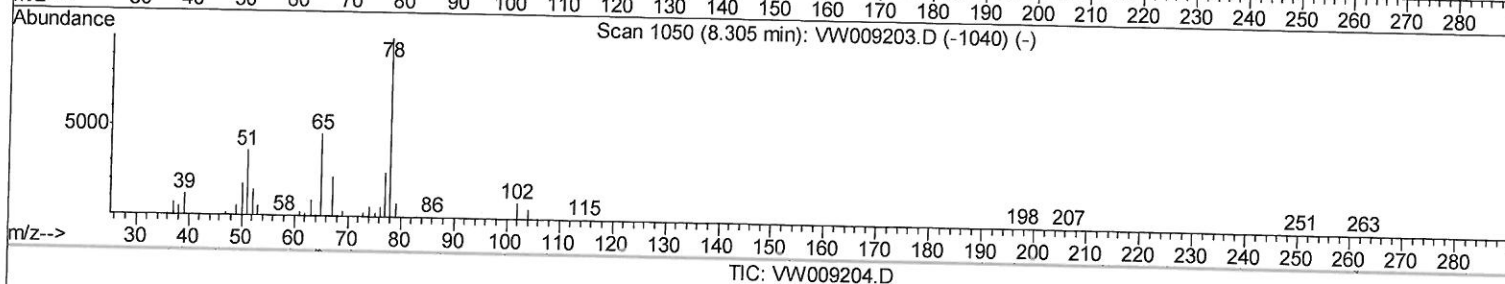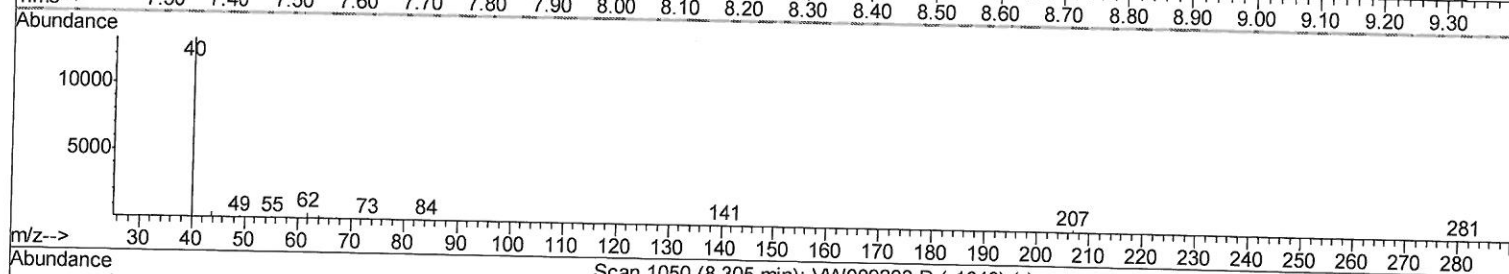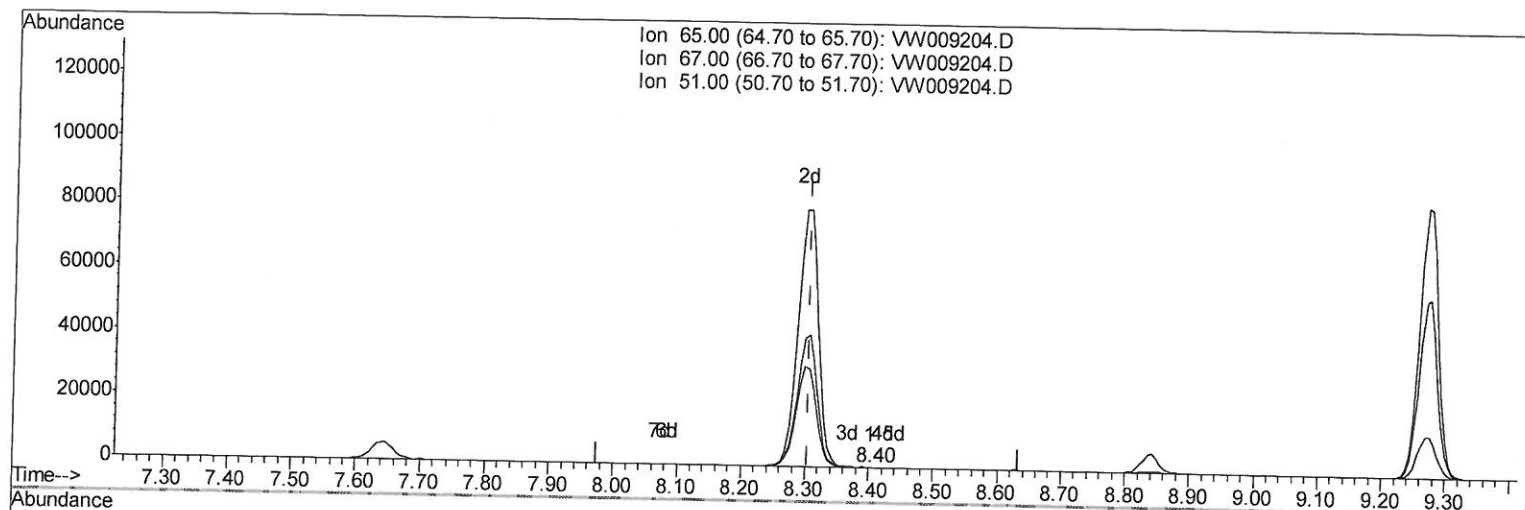

(26) 1,2-Dichloroethane-d4 (S)

8.402min (+0.097) 0.02ug/L

response 130

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	48.46
51.00	97.70	98.46
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW031619\
Quantitation Report (Qedit)




Data File : VW009204.D
Acq On : 16 Mar 2019 12:15
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK03

Manual Integrations
APPROVED

MMDadoda
3/19/2019 10:03:15 AM

Quant Time: Mar 18 02:43:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 02:40:38 2019
Response via : Initial Calibration

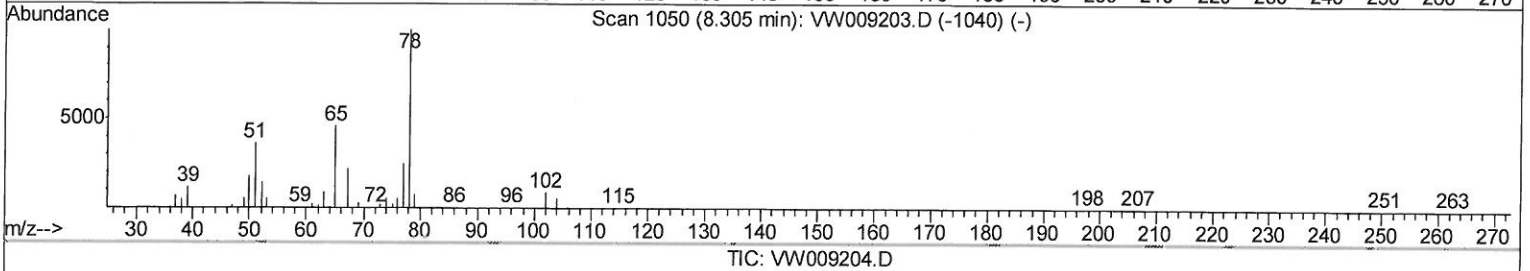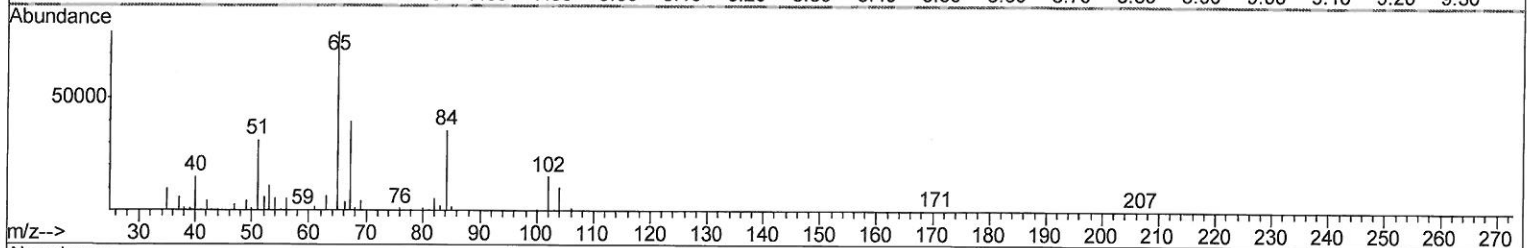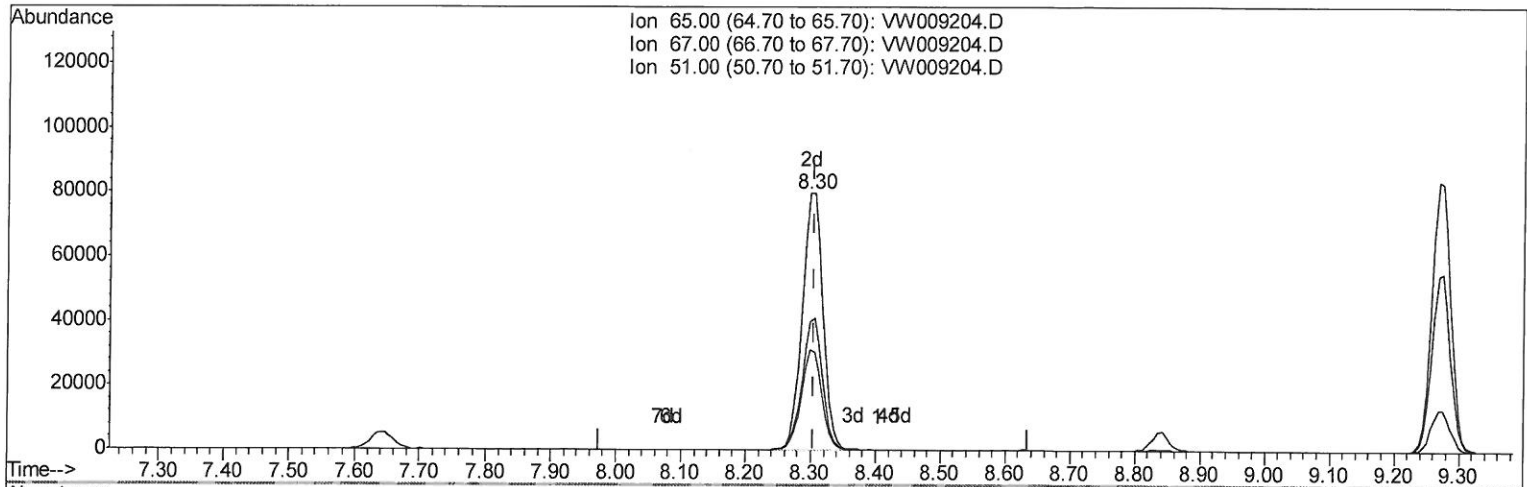

TIC: VW009204.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 22.41ug/L m

response 176464

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	0.04#
51.00	97.70	0.07#
0.00	0.00	0.00

> 03/18/19 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW031619\
Quantitation Report (QT/LSC Reviewed)

Data File : VW009204.D
Acq On : 16 Mar 2019 12:15
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleID :
VBLK03

Manual Integrations
APPROVED

MMDadoda
3/19/2019 10:03:15 AM

Quant Time: Mar 18 02:47:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 02:40:38 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	479010	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	457226	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	218820	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	137040	23.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.76%
7) Chloroethane-d5	2.89	69	131554	19.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.56%
10) 1,1-Dichloroethene-d2	4.01	63	207904	16.80	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.20%
20) 2-Butanone-d5	7.07	46	102581	43.33	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.66%
24) Chloroform-d	7.64	84	284510	21.76	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.04%
26) 1,2-Dichloroethane-d4	8.30	65	176464m	22.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.64%
29) Benzene-d6	8.27	84	555250	22.02	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.08%
33) 1,2-Dichloropropane-d6	9.27	67	168681	22.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.08%
37) Toluene-d8	10.32	98	513822	22.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.16%
38) trans-1,3-Dichloropropene-	10.58	79	80432	21.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.60%
39) 2-Hexanone-d5	10.93	63	78267	42.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	158538	21.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	194352	23.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.64%

03/18/19 dy

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed