
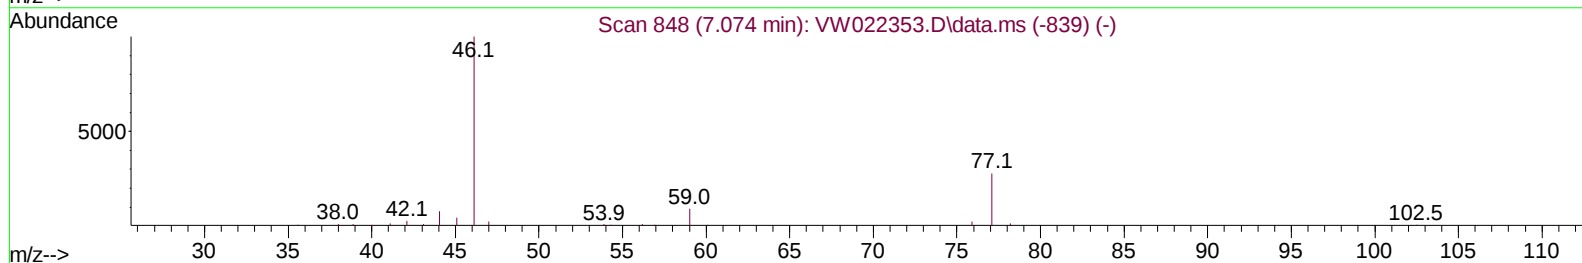
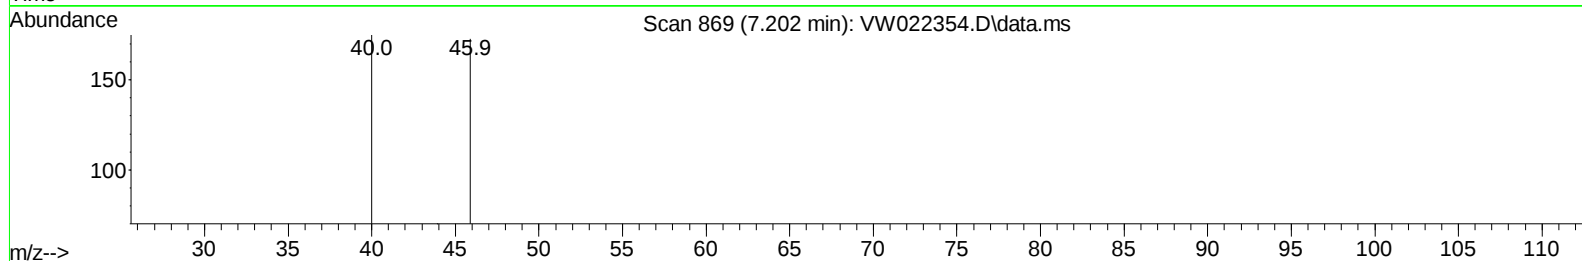


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022354.D
Acq On : 16 Mar 2022 13:19
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 17 00:17:26 2022
Response via : Initial Calibration

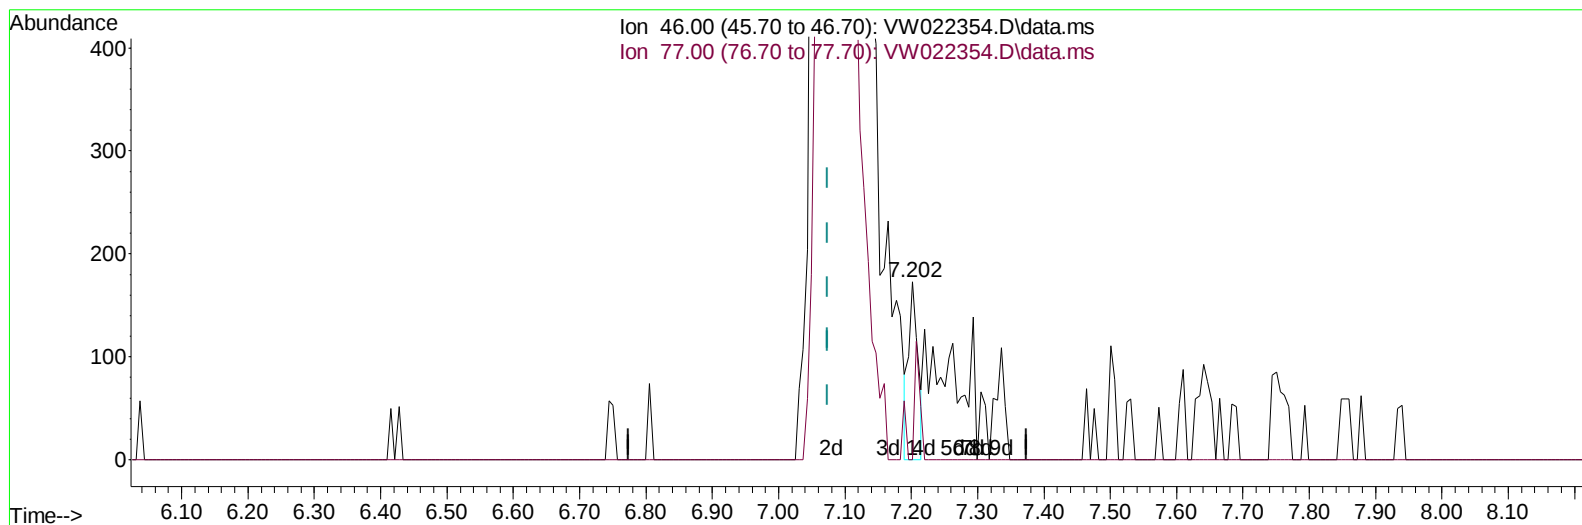

TIC: VW022354.D\data.ms

(21) 2-Butanone-d5 (S)




7.202min (+ 0.128) 0.59 ug/L

response 168

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	36.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022354.D
Acq On : 16 Mar 2022 13:19
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 17 00:17:26 2022
Response via : Initial Calibration

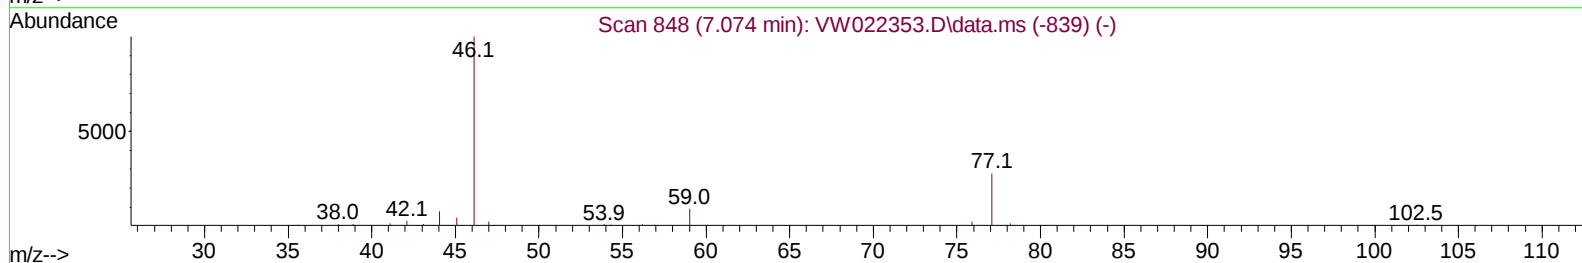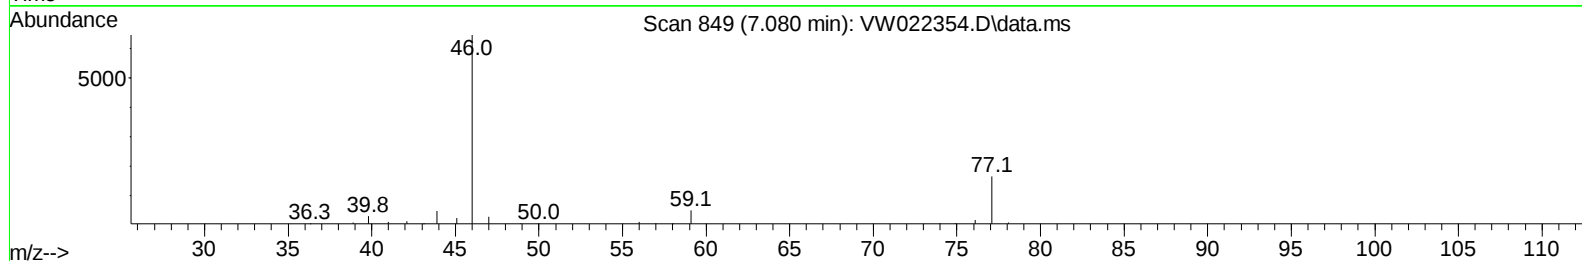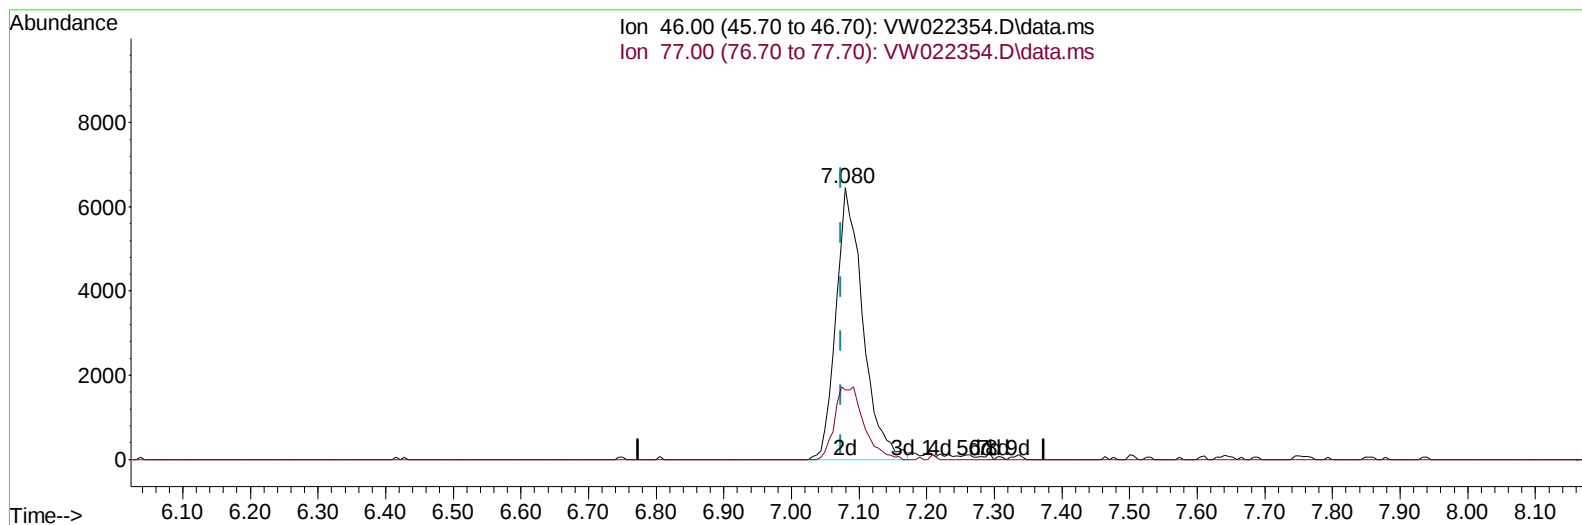

TIC: VW022354.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 62.03 ug/L m

response 17807

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	0.34#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
 Data File : VW022354.D
 Acq On : 16 Mar 2022 13:19
 Operator : SY/VA
 Sample : VW0316SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 17 00:17:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	130913	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	125750	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63951	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	36360	21.294	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.160%		
7) Chloroethane-d5	2.885	69	27863	20.739	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.960%		
11) 1,1-Dichloroethene-d2	4.013	63	39310	15.033	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.120%		
21) 2-Butanone-d5	7.080	46	17807m	62.025	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.060%		
24) Chloroform-d	7.647	84	71930	24.626	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	98.520%		
26) 1,2-Dichloroethane-d4	8.305	65	37635	24.788	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.160%		
32) Benzene-d6	8.275	84	131542	22.477	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.920%		
36) 1,2-Dichloropropane-d6	9.275	67	39017	24.006	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.040%		
41) Toluene-d8	10.323	98	126161	21.683	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.720%		
43) trans-1,3-Dichloroprop...	10.579	79	16344	22.680	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	90.720%		
47) 2-Hexanone-d5	10.921	63	14537	54.382	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.760%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	39732	27.855	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	111.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	53070	25.837	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.360%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022354.D
Acq On : 16 Mar 2022 13:19
Operator : SY/VA
Sample : VW0316SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 17 00:17:26 2022
Response via : Initial Calibration

