
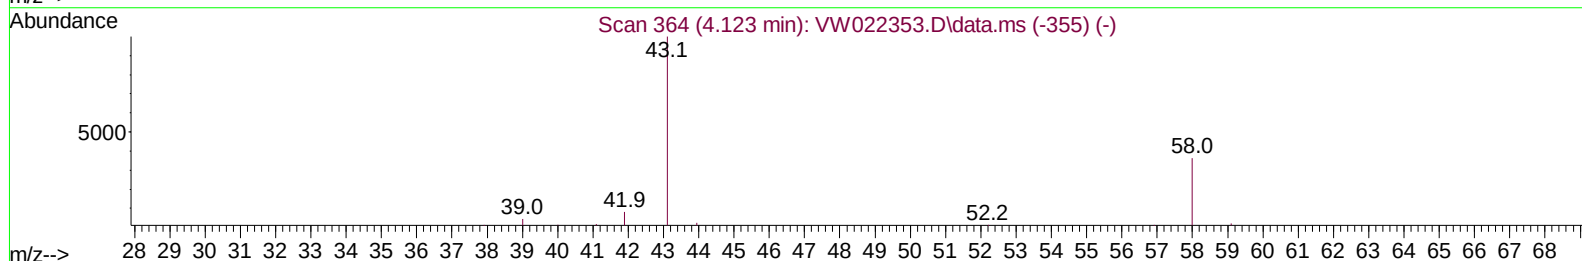
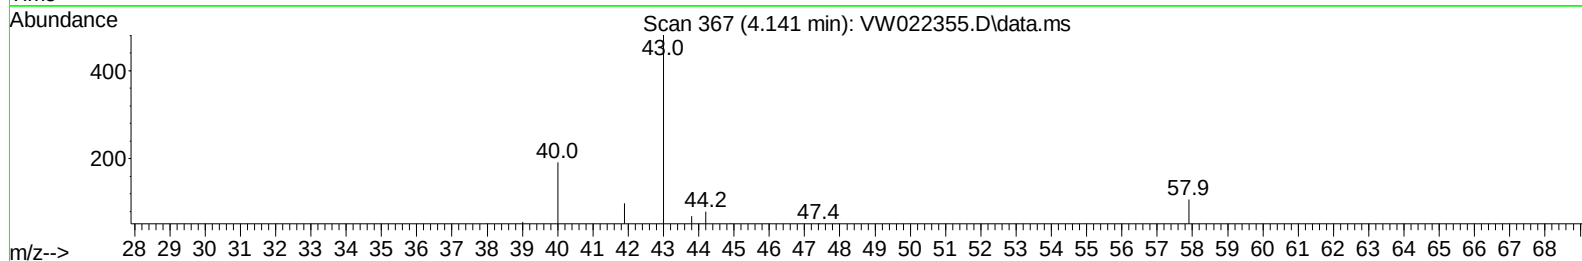


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022355.D
Acq On : 16 Mar 2022 13:43
Operator : SY/VA
Sample : N1883-06
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 17 00:17:26 2022
Response via : Initial Calibration

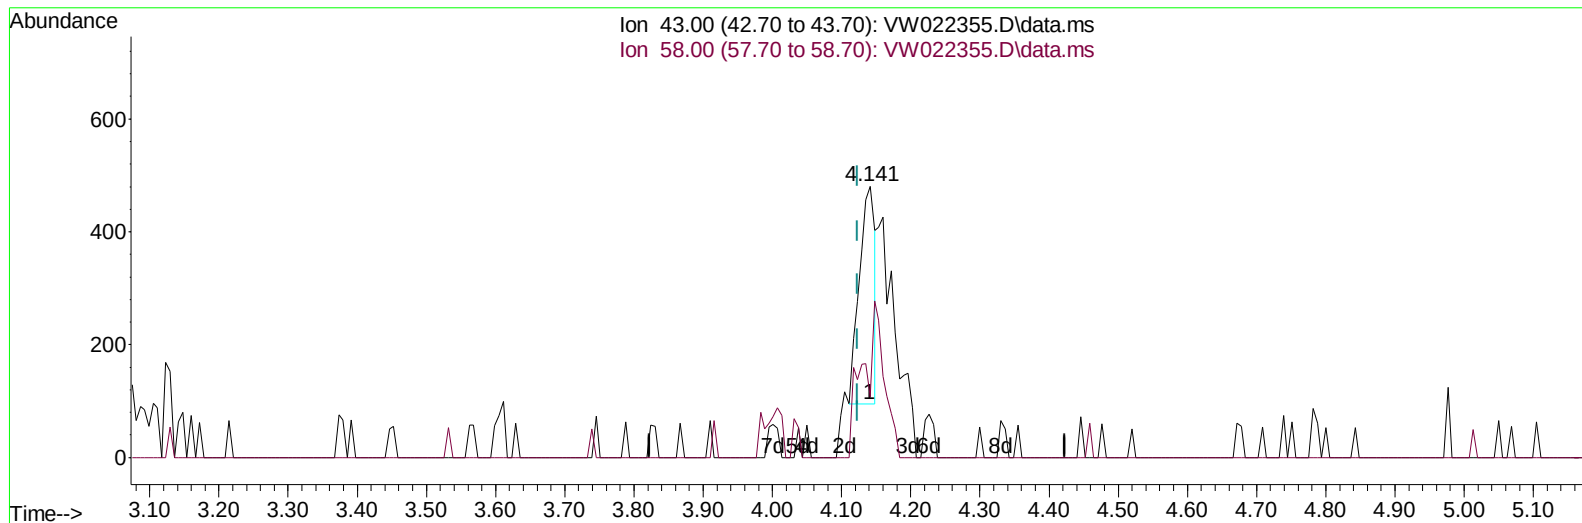

TIC: VW022355.D\data.ms

(13) Acetone (T)




4.141min (+ 0.018) 2.54 ug/L

response 595

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
 Data File : VW022355.D
 Acq On : 16 Mar 2022 13:43
 Operator : SY/VA
 Sample : N1883-06
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 17 00:17:26 2022
 Response via : Initial Calibration

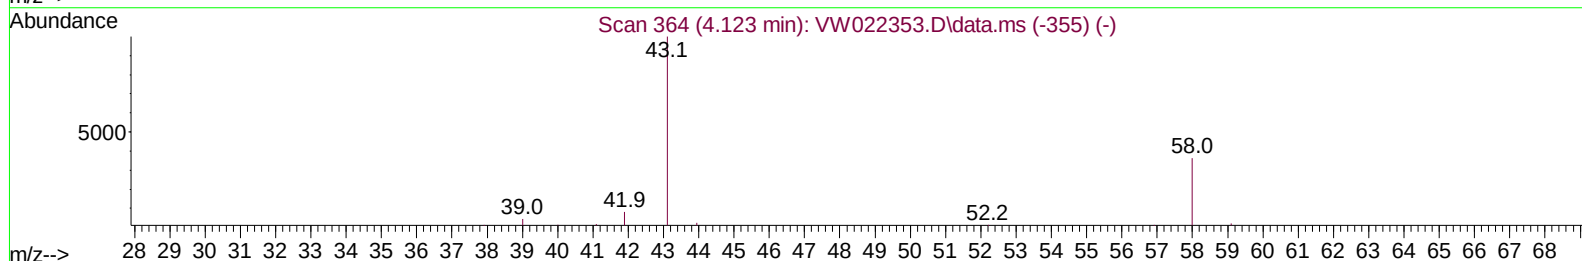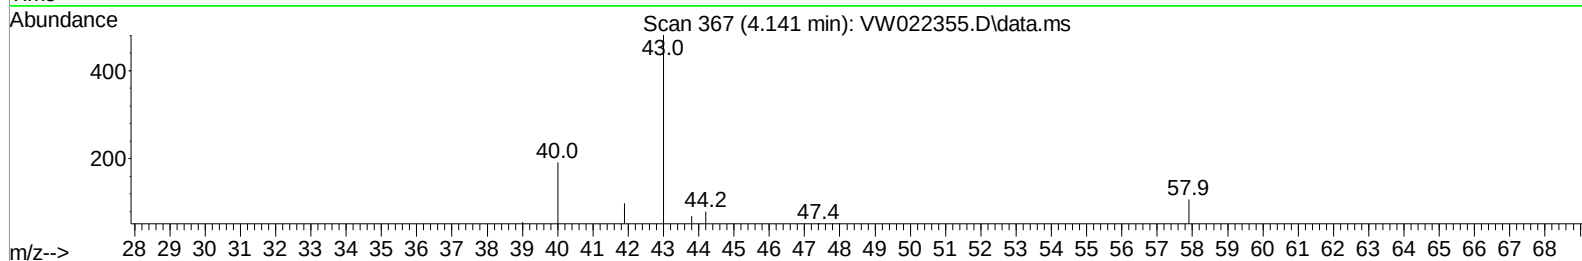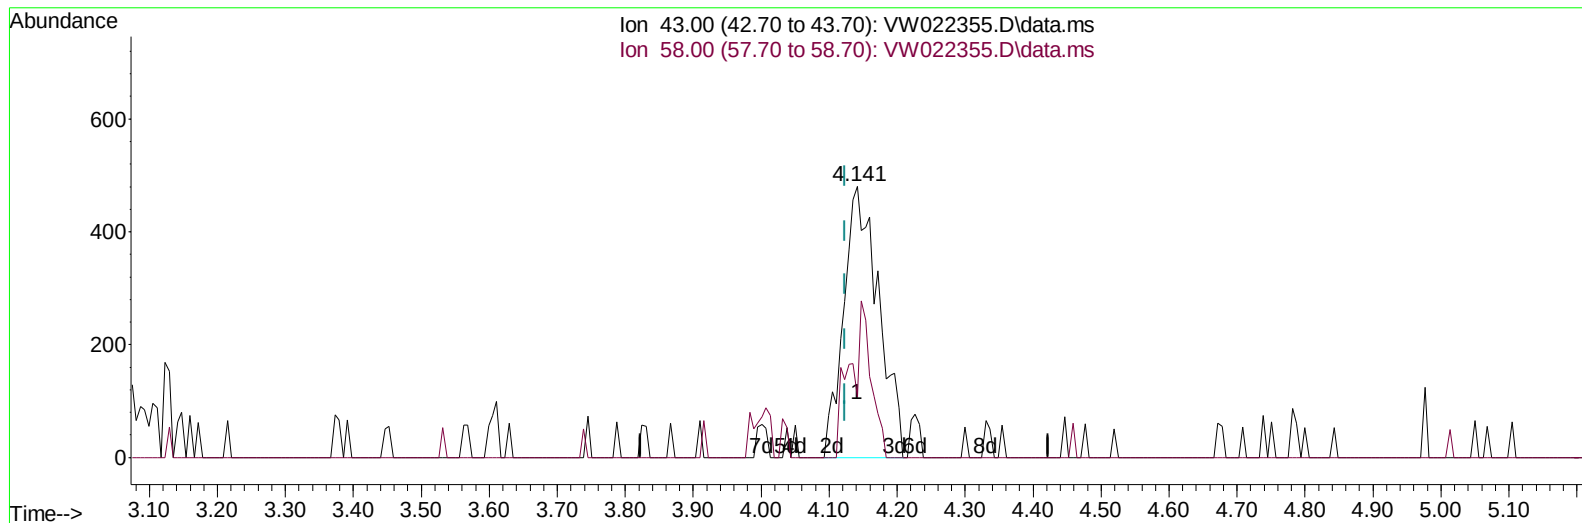

TIC: VW022355.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 7.27 ug/L m

response 1706

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	9.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
 Data File : VW022355.D
 Acq On : 16 Mar 2022 13:43
 Operator : SY/VA
 Sample : N1883-06
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Mar 17 00:17:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	130988	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	122920	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	56835	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	34279	20.064	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.240%	
7) Chloroethane-d5	2.879	69	26301	19.565	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.280%	
11) 1,1-Dichloroethene-d2	4.013	63	36103	13.799	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.200%	
21) 2-Butanone-d5	7.080	46	17322	60.301	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.600%	
24) Chloroform-d	7.647	84	62348	21.334	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.320%	
26) 1,2-Dichloroethane-d4	8.305	65	33851	22.283	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.120%	
32) Benzene-d6	8.275	84	113497	19.840	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	79.360%	
36) 1,2-Dichloropropane-d6	9.275	67	34001	21.402	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.600%	
41) Toluene-d8	10.323	98	104130	18.309	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.240%	
43) trans-1,3-Dichloroprop...	10.579	79	13665	19.399	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.600%	
47) 2-Hexanone-d5	10.921	63	13101	50.139	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.280%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	35716	25.616	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	42336	23.192	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.760%	
Target Compounds						
13) Acetone	4.141	43	1706m	7.271	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022355.D
Acq On : 16 Mar 2022 13:43
Operator : SY/VA
Sample : N1883-06
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 00:19:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Mar 17 00:17:26 2022
Response via : Initial Calibration

