
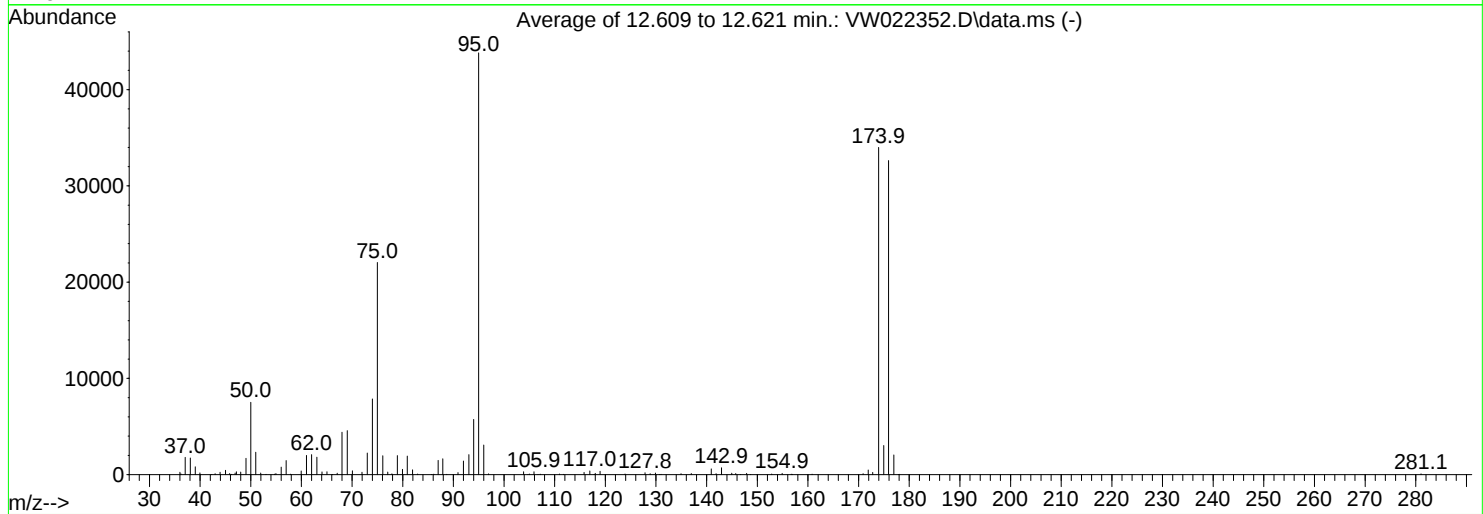


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031622\
Data File : VW022352.D
Acq On : 16 Mar 2022 10:10
Operator : SY/VA
Sample : BFB524
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB524

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Title : SFAM01.0
Last Update : Thu Mar 17 00:17:26 2022

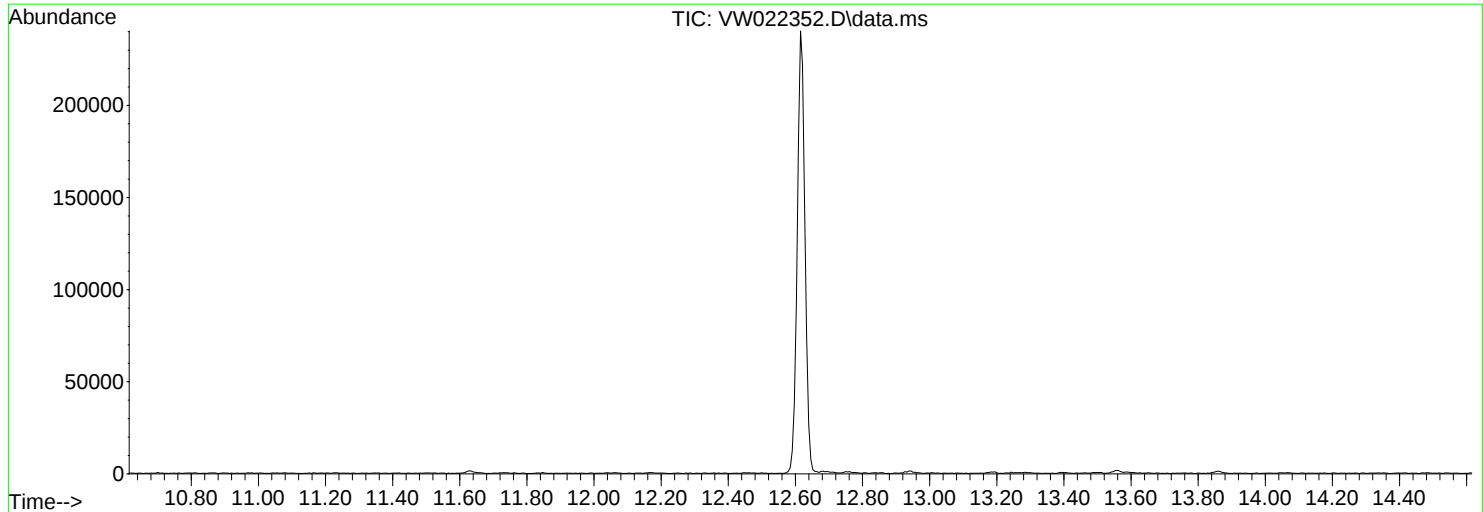

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	7515	PASS
75	95	30	80	50.3	22043	PASS
95	95	100	100	100.0	43824	PASS
96	95	5	9	7.0	3068	PASS
173	174	0.00	2	0.7	236	PASS
174	95	50	120	77.6	33989	PASS
175	174	5	9	8.9	3021	PASS
176	174	95	105	96.0	32635	PASS
177	176	5	10	6.3	2051	PASS

m/z	Abundance
40.10	212.0
44.00	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB524

m/z	Abundance
36.00	342.0
37.10	1787.0
38.00	1574.0
39.10	803.0
40.00	170.0
43.00	113.0
44.00	310.0
45.00	479.0
45.90	120.0
47.10	392.0
48.00	303.0
49.00	1642.0
50.00	6887.0
51.00	2231.0
51.90	118.0
53.00	110.0
54.70	150.0
56.00	686.0
57.00	1306.0
57.90	81.0
60.00	355.0
61.00	1828.0
62.00	1875.0
63.00	1594.0
64.00	288.0
65.00	327.0
66.10	67.0
67.10	154.0
68.00	4058.0
69.10	3918.0
70.00	362.0
72.00	237.0
73.00	1896.0
74.00	6795.0
75.00	19280.0
76.00	1598.0
77.10	246.0
77.90	106.0
79.00	1736.0
80.00	465.0
80.90	1684.0
82.00	378.0
83.00	76.0
86.10	50.0
87.00	1040.0
87.90	1324.0
88.70	123.0
90.90	183.0
92.00	1145.0
93.10	1615.0
94.00	4738.0
95.00	38152.0
96.00	2310.0
97.00	105.0
103.90	222.0
104.70	72.0
105.90	201.0
106.70	71.0
111.70	69.0
115.80	177.0
117.00	325.0
117.80	128.0
119.00	313.0
123.90	55.0
127.80	144.0
128.90	88.0
129.80	88.0
131.00	50.0
134.90	78.0
136.90	122.0
140.90	507.0
141.80	82.0
142.90	721.0
145.00	130.0
145.80	58.0
146.70	59.0
147.80	125.0
152.90	58.0
155.00	114.0
156.70	62.0
171.00	91.0
171.90	410.0
172.80	709.0
173.90	28544.0
174.90	2463.0
175.90	23248.0
177.00	1379.0
281.10	162.0

Instrument :
MSVOA_W
ClientSampleId :
BFB524

m/z	Abundance
36.00	383.0
37.00	1976.0
38.00	2248.0
39.10	906.0
39.80	148.0
40.20	103.0
42.90	82.0
43.90	461.0
45.00	456.0
45.80	145.0
47.20	518.0
48.00	279.0
49.00	1712.0
50.00	8360.0
51.00	2679.0
52.00	144.0
54.90	140.0
56.00	890.0
57.00	1593.0
57.80	68.0
60.00	335.0
61.00	2280.0
62.00	2353.0
63.00	2046.0
64.10	263.0
65.10	317.0
67.00	271.0
68.00	4807.0
69.00	5177.0
70.10	381.0
72.00	238.0
73.00	2593.0
74.00	8745.0
75.00	24488.0
76.10	2405.0
77.00	272.0
78.90	2192.0
79.90	689.0
80.90	2140.0
82.00	577.0
82.90	62.0
85.70	58.0
86.20	86.0
87.00	1669.0
87.90	2067.0
90.80	214.0
92.00	1613.0
93.00	2457.0
94.00	6489.0
95.00	49976.0
96.00	3801.0
96.90	92.0
103.90	312.0
105.00	92.0
105.90	316.0
107.20	100.0
111.00	111.0
111.80	52.0
115.80	258.0
116.90	468.0
118.00	201.0
118.90	356.0
123.90	78.0
127.90	230.0
128.90	98.0
129.90	232.0
130.70	63.0
135.00	152.0
137.00	126.0
141.00	731.0
141.90	141.0
143.00	674.0
145.00	173.0
145.70	166.0
147.90	182.0
152.90	73.0
155.00	120.0
156.70	70.0
160.80	67.0
170.80	126.0
171.90	506.0
174.00	35088.0
174.90	3322.0
175.90	38968.0
176.90	2124.0
177.90	76.0
281.00	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB524

m/z	Abundance
36.20	270.0
37.00	1603.0
38.10	1353.0
39.00	725.0
40.00	234.0
42.30	69.0
42.90	90.0
43.90	397.0
45.00	399.0
45.80	84.0
46.20	81.0
46.90	522.0
48.00	240.0
49.10	1757.0
50.00	7299.0
51.00	2096.0
51.90	220.0
55.00	194.0
56.00	769.0
57.00	1474.0
59.90	483.0
61.00	1872.0
62.00	1997.0
63.10	1780.0
64.00	277.0
65.00	273.0
68.00	4370.0
69.00	4613.0
70.00	432.0
71.90	267.0
73.00	2243.0
74.00	8074.0
75.00	22360.0
76.00	1860.0
77.00	303.0
77.80	154.0
78.90	2003.0
79.90	475.0
80.90	1980.0
81.90	531.0
82.90	68.0
87.00	1759.0
87.90	1536.0
91.00	236.0
92.00	1502.0
93.00	2185.0
94.00	5999.0
95.00	43344.0
96.00	3093.0
96.90	74.0
103.80	367.0
105.00	96.0
105.90	378.0
107.00	55.0
110.90	113.0
115.80	245.0
116.90	358.0
118.00	223.0
118.90	384.0
123.90	66.0
127.90	240.0
128.80	111.0
130.00	162.0
131.00	78.0
135.00	94.0
136.90	123.0
140.80	580.0
141.90	67.0
143.00	734.0
144.80	135.0
145.80	111.0
148.00	97.0
148.70	51.0
152.70	51.0
154.80	187.0
156.90	86.0
160.80	81.0
170.90	67.0
171.90	537.0
173.90	38336.0
175.00	3278.0
175.90	35688.0
176.90	2649.0
178.10	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB524