
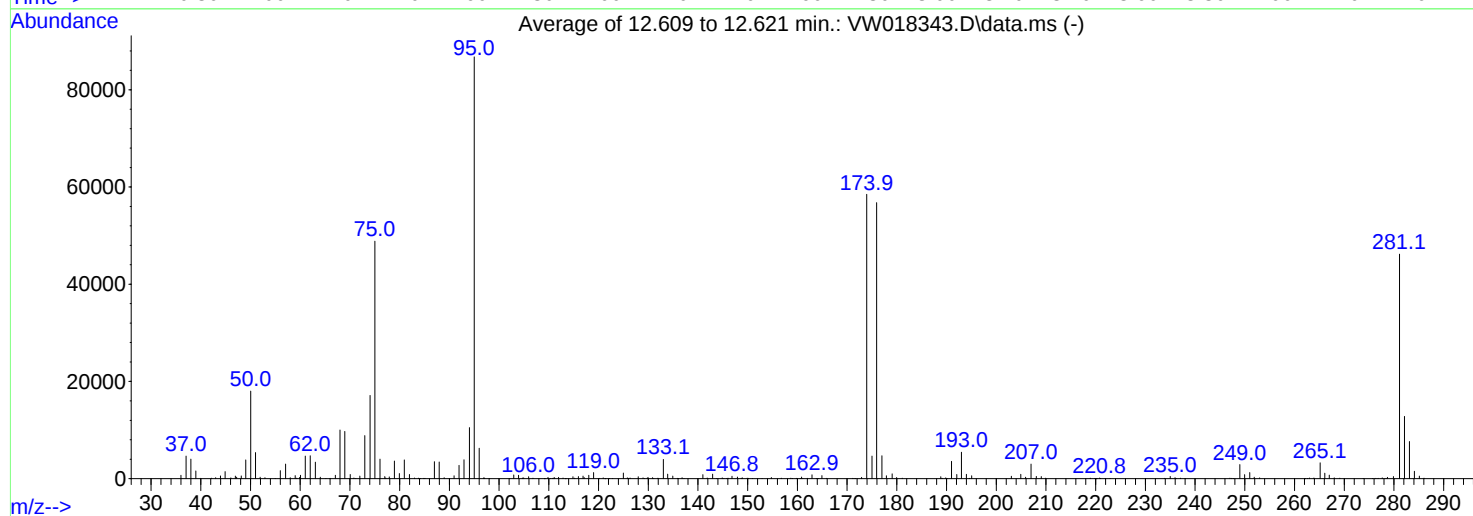


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031721\
 Data File : VW018343.D
 Acq On : 17 Mar 2021 13:03
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W031721S.M
 Title : SW846 8260
 Last Update : Wed Mar 17 18:51:14 2021

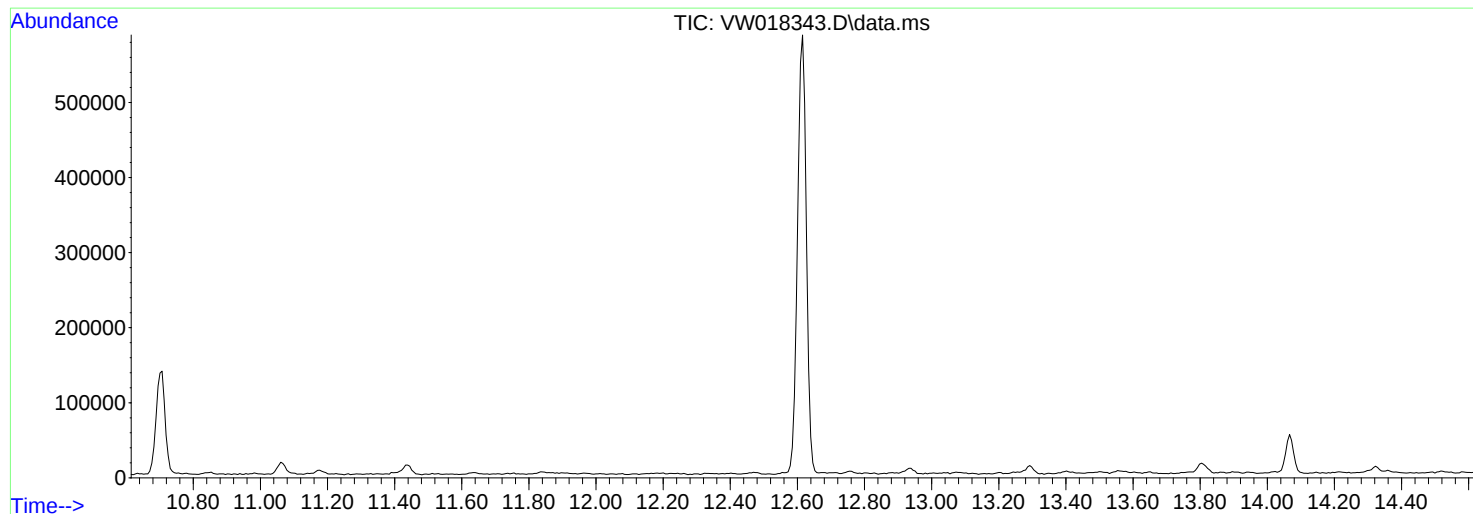

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	17994	PASS
75	95	30	60	56.3	48851	PASS
95	95	100	100	100.0	86784	PASS
96	95	5	9	7.2	6267	PASS
173	174	0.00	2	0.5	281	PASS
174	95	50	100	67.4	58488	PASS
175	174	5	9	7.9	4642	PASS
176	174	95	101	97.1	56789	PASS
177	176	5	9	8.3	4715	PASS