

Data File : VW009230.D
Acq On : 18 Mar 2019 15:36
Operator : SY/VA
Sample : K1936-19
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Mar 19 01:34:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 19 01:10:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	425487	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	410140	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	194090	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	133081	26.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.68%
7) Chloroethane-d5	2.89	69	127650	21.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.84%
10) 1,1-Dichloroethene-d2	4.01	63	208439	18.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.88%
20) 2-Butanone-d5	7.07	46	89020	42.33	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.66%
24) Chloroform-d	7.65	84	278792	24.01	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.04%
26) 1,2-Dichloroethane-d4	8.31	65	167934	24.01	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.04%
29) Benzene-d6	8.27	84	528576	23.37	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.48%
33) 1,2-Dichloropropane-d6	9.27	67	161484	23.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.08%
37) Toluene-d8	10.32	98	480643	22.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.92%
38) trans-1,3-Dichloropropene-	10.57	79	73598	21.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.28%
39) 2-Hexanone-d5	10.93	63	64336	39.10	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.20%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	144038	21.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.12%
61) 1,2-Dichlorobenzene-d4	13.86	152	184833	24.83	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.32%


Target Compounds					Qvalue
42) cis-1,3-Dichloropropene	10.03	75	5950	0.634 ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW009230.D
Acq On : 18 Mar 2019 15:36
Operator : SY/VA
Sample : K1936-19
Misc : 5.03G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Mar 19 01:34:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 19 01:10:50 2019
Response via : Initial Calibration

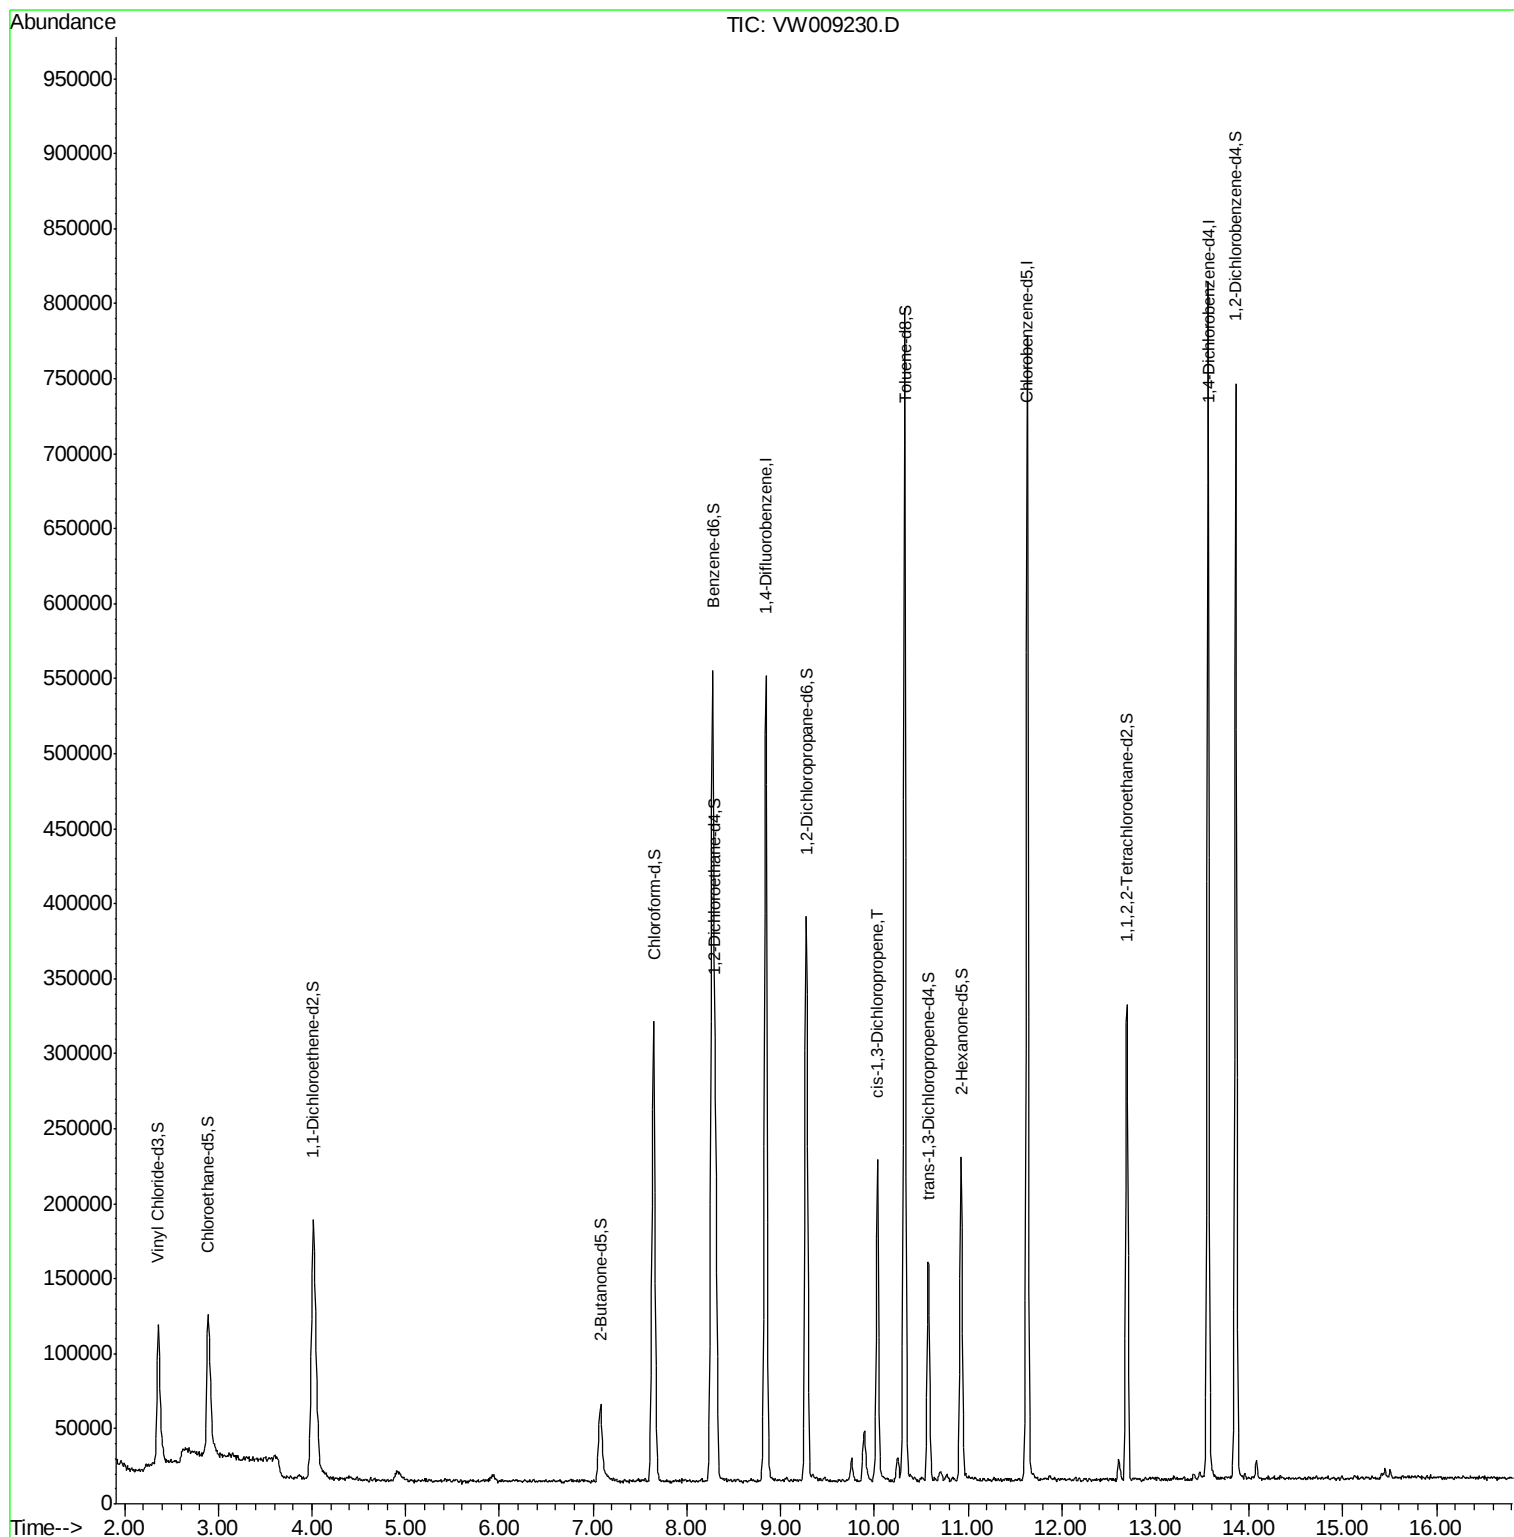

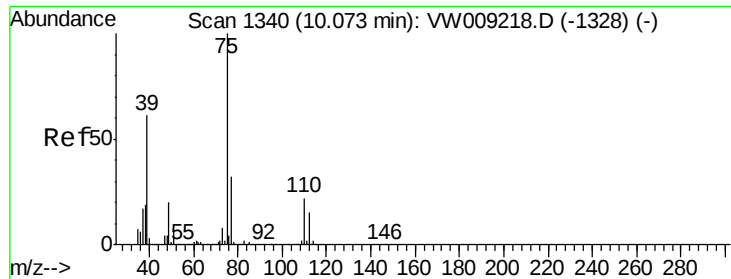

#42

cis-1,3-Dichloropropene

Concen: 0.634 ug/L

RT: 10.03 min Scan# 1333

Delta R.T. -0.04 min

Lab File: VW009230.D

Acq: 18 Mar 2019 15:36

Instrument :

MSVOA_W

ClientSampleId :

VHBLK01

Tgt Ion: 75 Resp: 5950

Ion Ratio Lower Upper

75 100

77 41.4 21.6 40.2#

