

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031819\
Quantitation Report (QT Reviewed)


Data File : VW009219.D
Acq On : 18 Mar 2019 09:54
Operator : SY/VA
Sample : VW0318SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK04

Manual Integrations
APPROVED

MMDadoda
3/20/2019 9:18:42 AM

Quant Time: Mar 18 11:15:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 11:10:57 2019
Response via : Initial Calibration

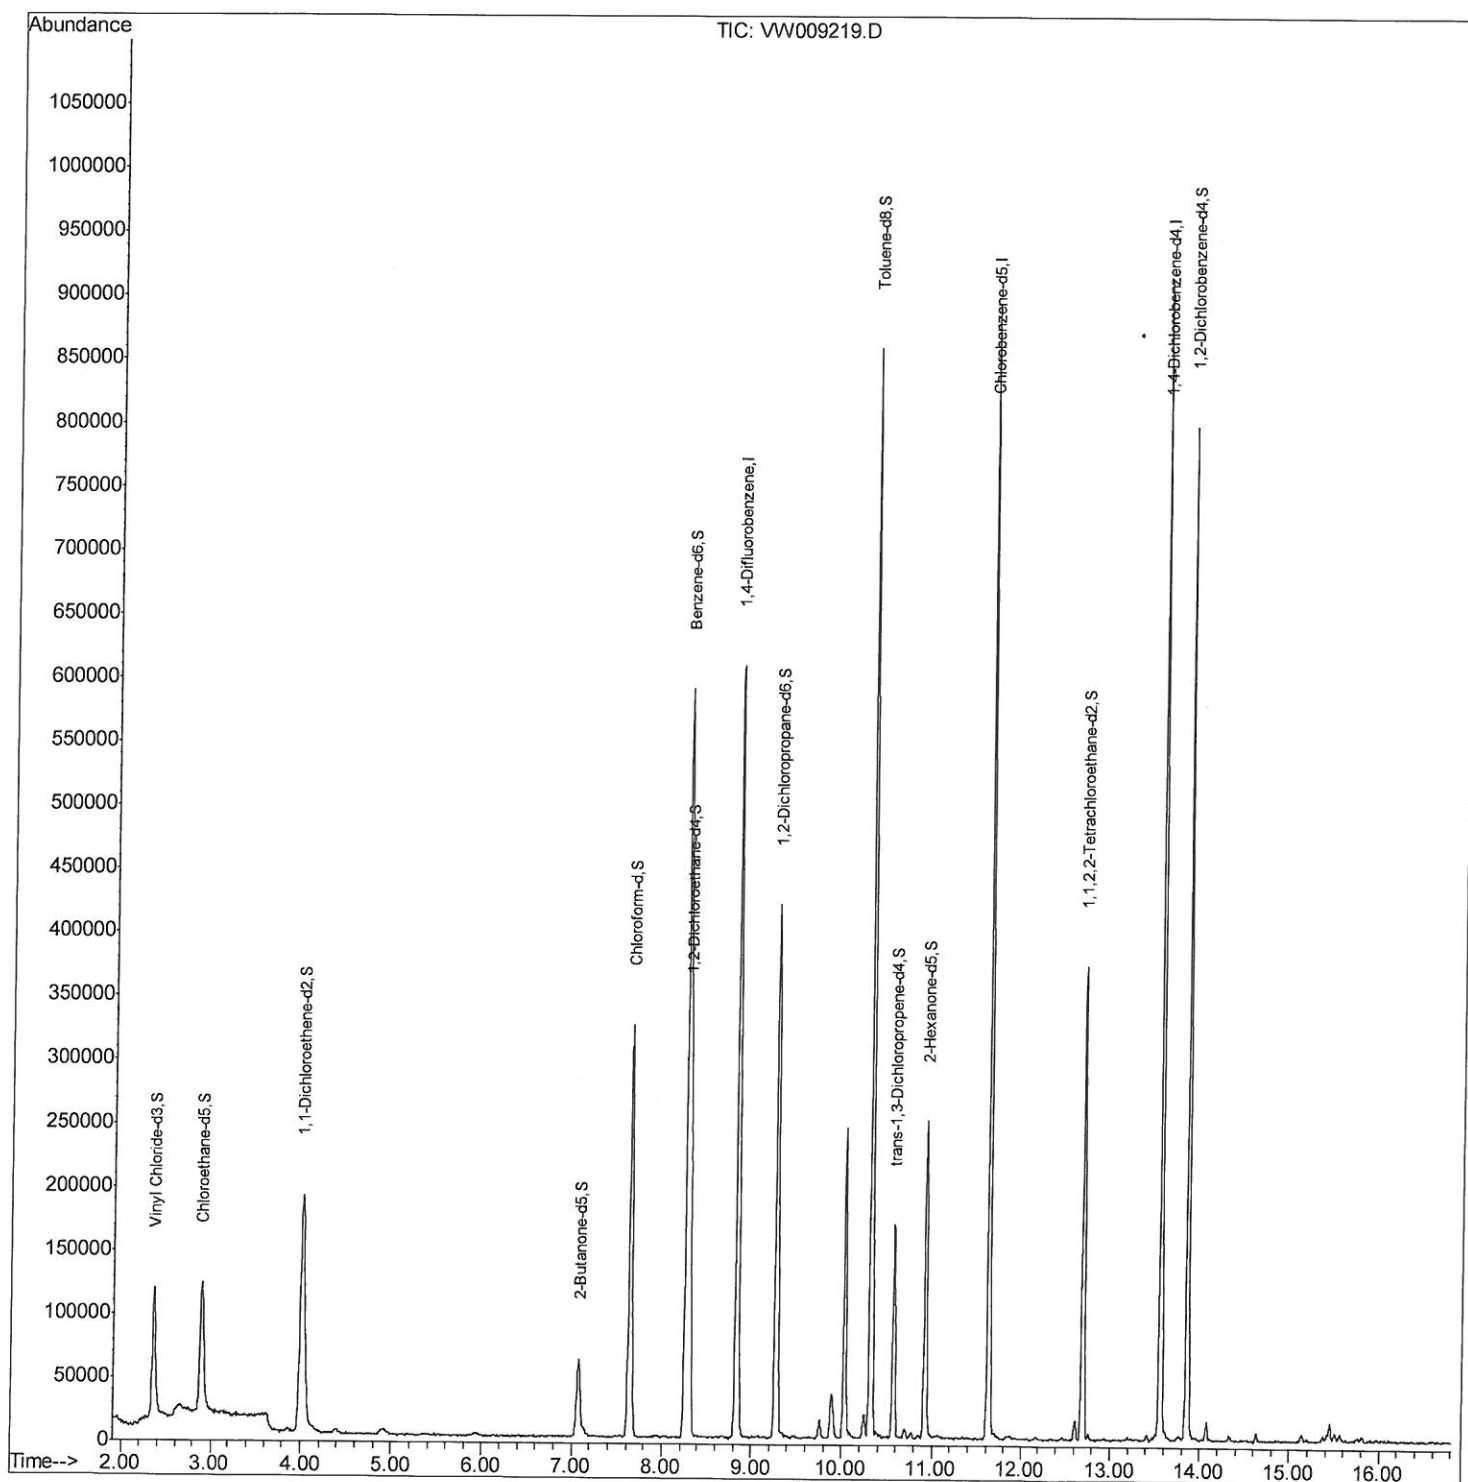

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031819\
Quantitation Report (Qedit)




Data File : VW009219.D
Acq On : 18 Mar 2019 09:54
Operator : SY/VA
Sample : VW0318SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK04

Manual Integrations
APPROVED

MMDadoda
3/20/2019 9:18:42 AM

Quant Time: Mar 18 11:13:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 11:10:57 2019
Response via : Initial Calibration

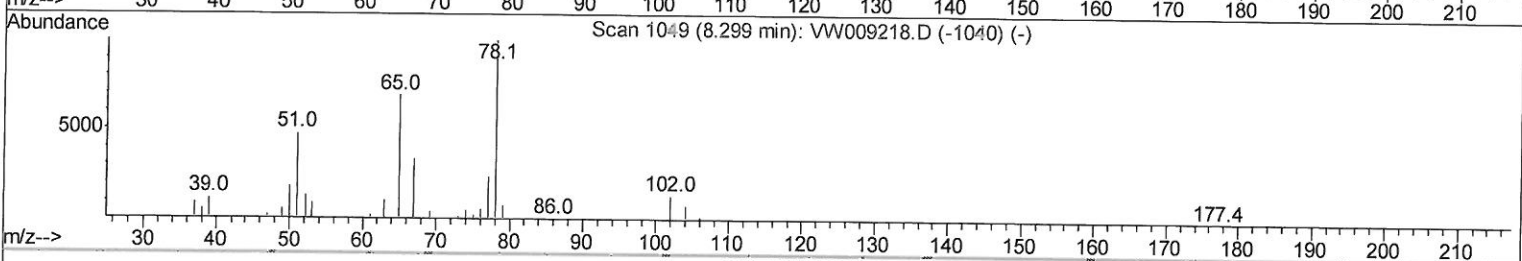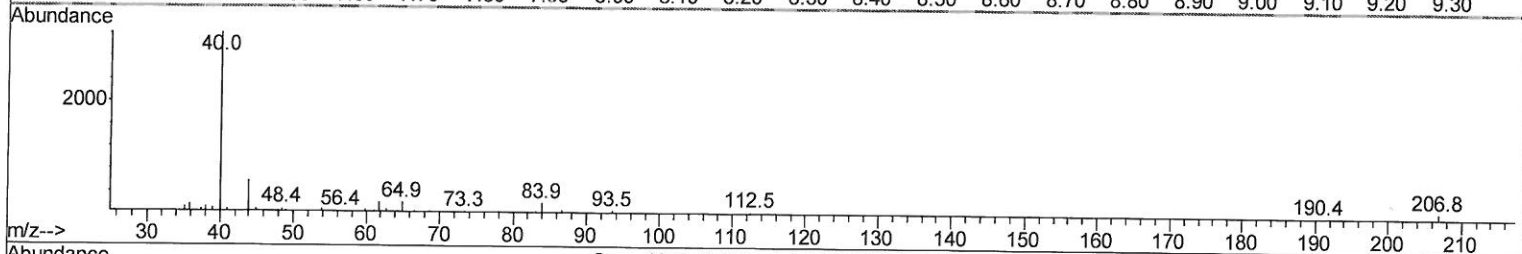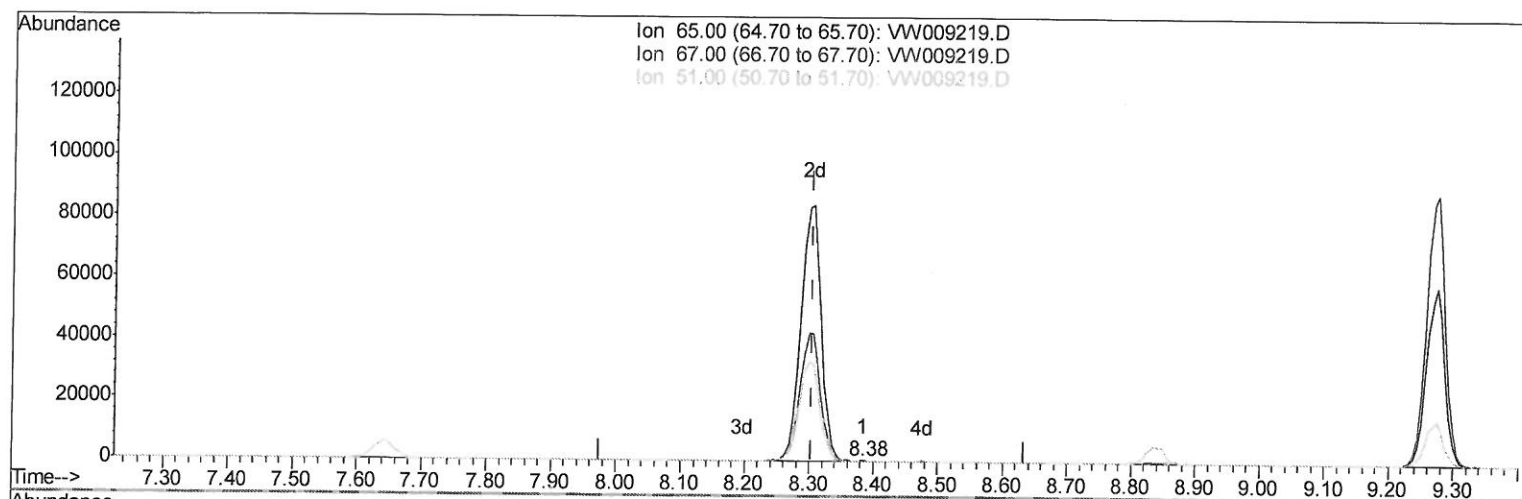

TIC: VW009219.D

(26) 1,2-Dichloroethane-d4 (S)

8.384min (+0.079) 0.01ug/L

response 84

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	44.05
51.00	97.70	101.19
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031819\
Quantitation Report (Qedit)




Data File : VW009219.D
Acq On : 18 Mar 2019 09:54
Operator : SY/VA
Sample : VW0318SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK04

Manual Integrations
APPROVED

MMDadoda
3/20/2019 9:18:42 AM

Quant Time: Mar 18 11:13:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 11:10:57 2019
Response via : Initial Calibration

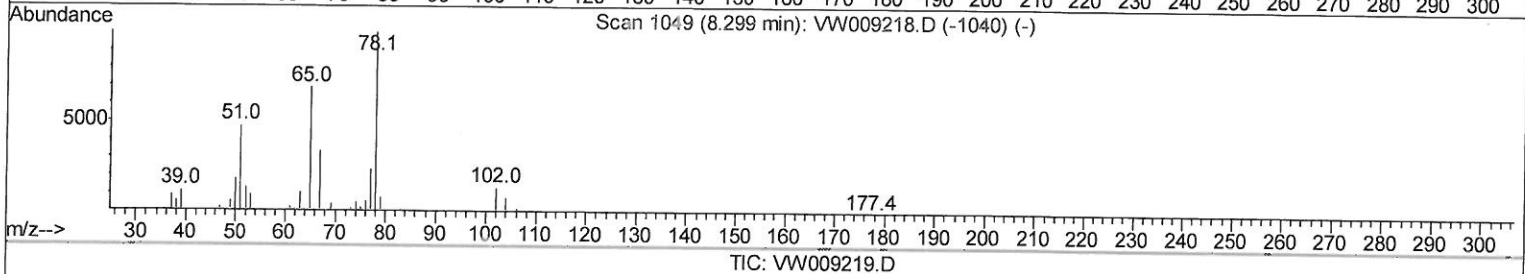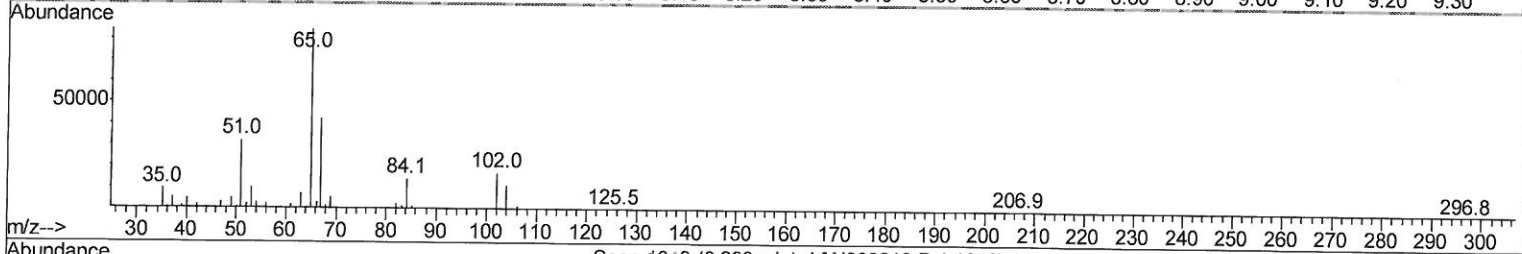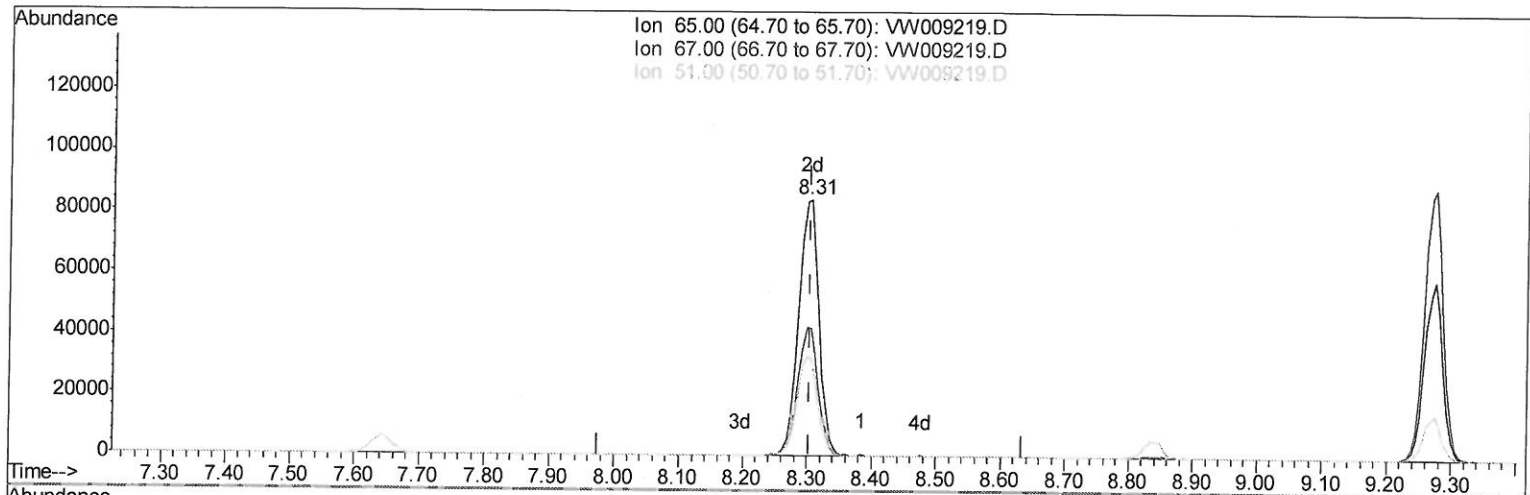

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 22.75ug/L m

response 184386

Ion Exp% Act%

65.00 100 100

67.00 50.80 0.02#

51.00 97.70 0.05#

0.00 0.00 0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031819\
Quantitation Report (QT Reviewed)

Data File : VW009219.D
Acq On : 18 Mar 2019 09:54
Operator : SY/VA
Sample : VW0318SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK04

Manual Integrations
APPROVED

MMDadoda
3/20/2019 9:18:42 AM

Quant Time: Mar 18 11:15:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 11:10:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	493041	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	464029	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	223459	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	148007	25.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.48%
7) Chloroethane-d5	2.89	69	140456	20.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.48%
10) 1,1-Dichloroethene-d2	4.01	63	227852	17.89	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.56%
20) 2-Butanone-d5	7.07	46	103823	42.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.22%
24) Chloroform-d	7.64	84	302219	22.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.84%
26) 1,2-Dichloroethane-d4	8.31	65	184386m	22.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.00%
29) Benzene-d6	8.27	84	583711	22.81	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.24%
33) 1,2-Dichloropropane-d6	9.27	67	175556	22.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.36%
37) Toluene-d8	10.32	98	535765	22.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.56%
38) trans-1,3-Dichloropropene-	10.57	79	84295	21.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.36%
39) 2-Hexanone-d5	10.92	63	78307	42.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	162850	21.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	205514	23.98	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.92%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/19/19 Sy