

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031821\
 Data File : VW018362.D
 Acq On : 18 Mar 2021 10:36
 Operator : SY/VA
 Sample : VD0318SBL01
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VD0318SBL01

Quant Time: Mar 18 16:40:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W031721S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 17 18:51:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.945	168	358392	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.841	114	586162	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.633	117	540682	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.554	152	248318	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.305	65	197630	51.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.28%	
35) Dibromofluoromethane	7.884	113	171826	50.30	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.60%	
50) Toluene-d8	10.323	98	696090	51.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.48%	
62) 4-Bromofluorobenzene	12.615	95	251278	48.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.46%	


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031821\
Data File : VW018362.D
Acq On : 18 Mar 2021 10:36
Operator : SY/VA
Sample : VD0318SBL01
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VD0318SBL01

Quant Time: Mar 18 16:40:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W031721S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 17 18:51:14 2021
Response via : Initial Calibration




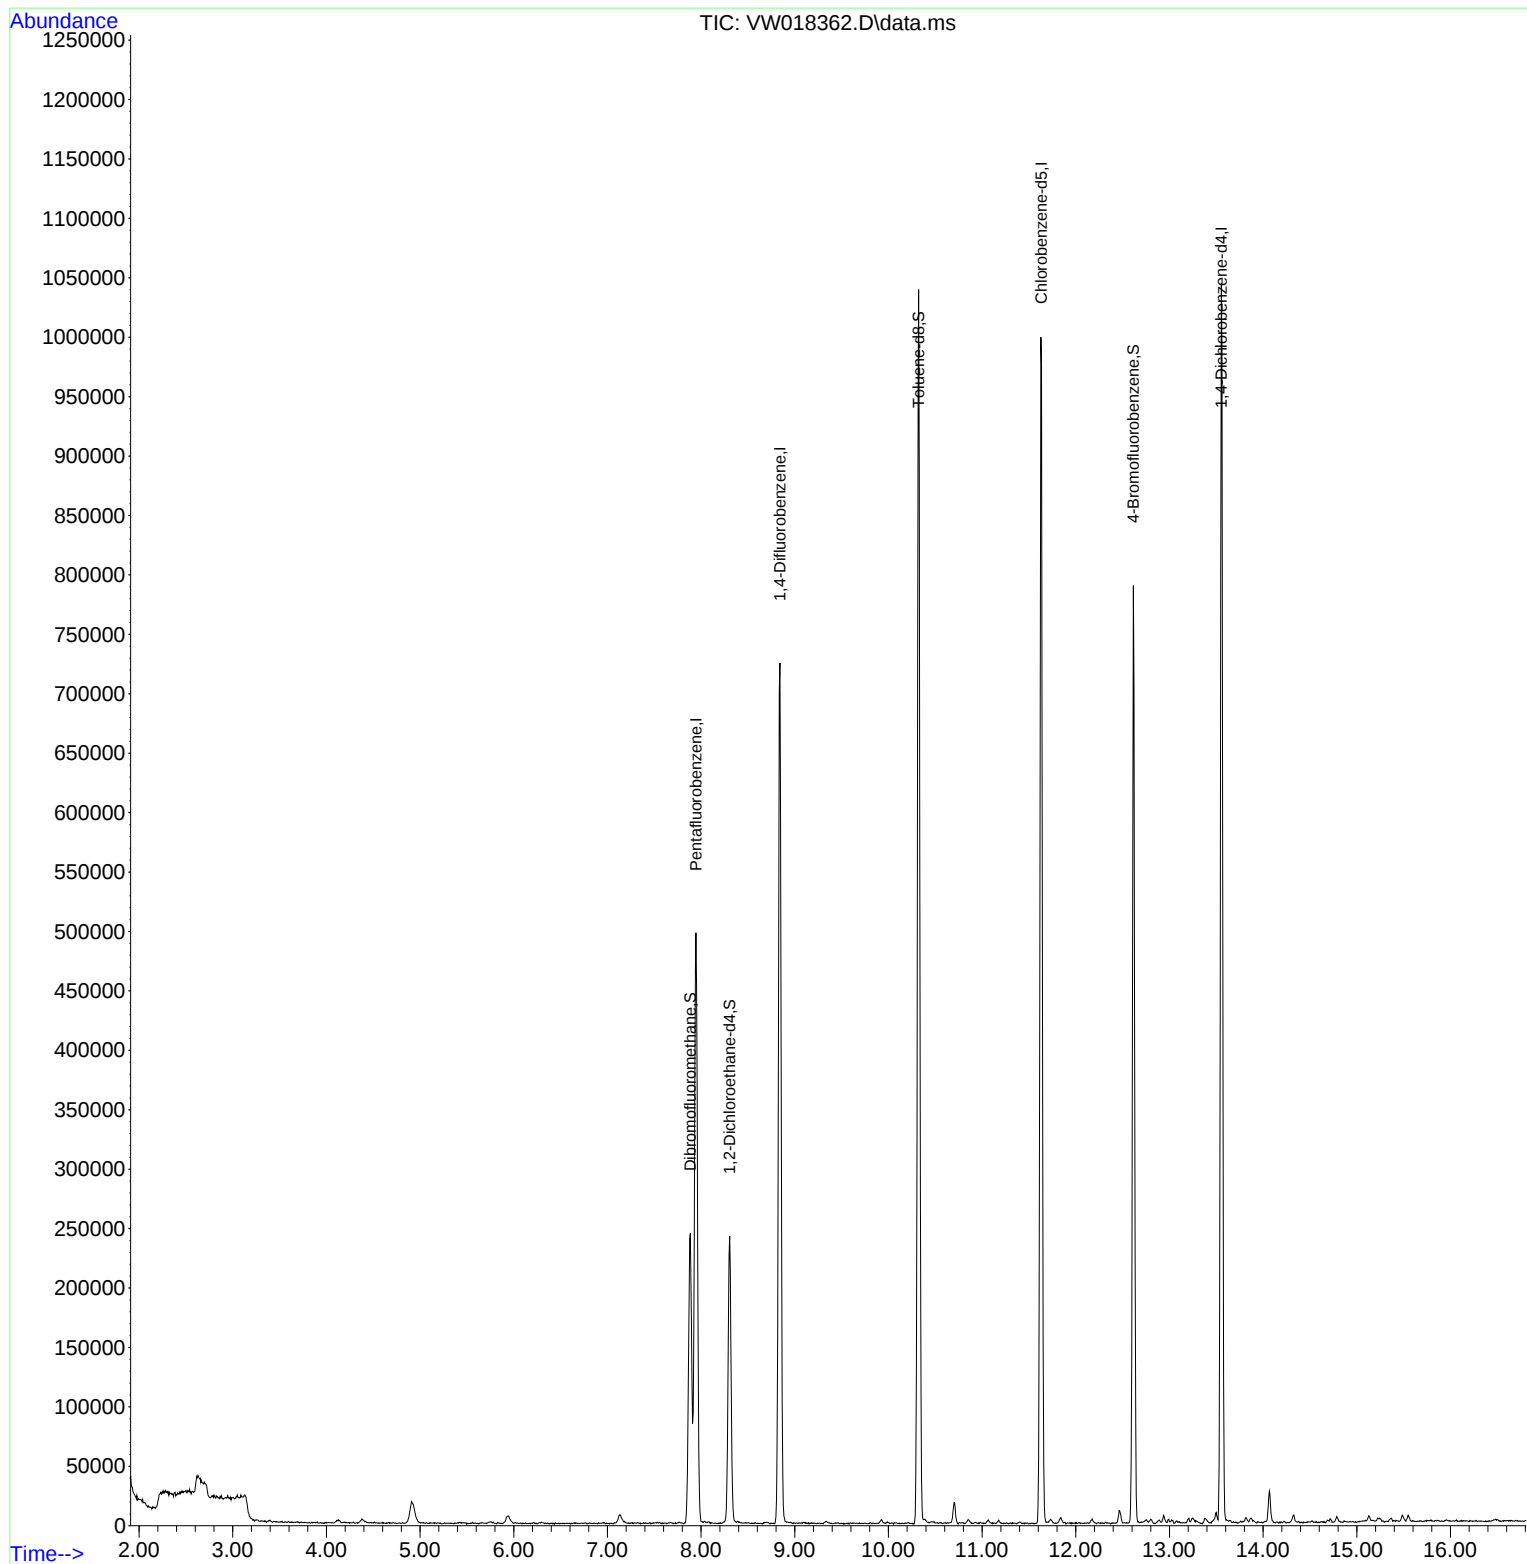


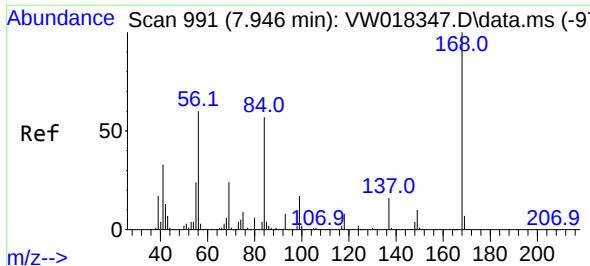

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.945 min Scan# 991
Delta R.T. -0.001 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36




Instrument :
MSVOA_W
ClientSampleId :
VD0318SBL01


Tgt Ion:168 Resp: 358392
Ion Ratio Lower Upper
168 100
99 70.2 60.8 91.2

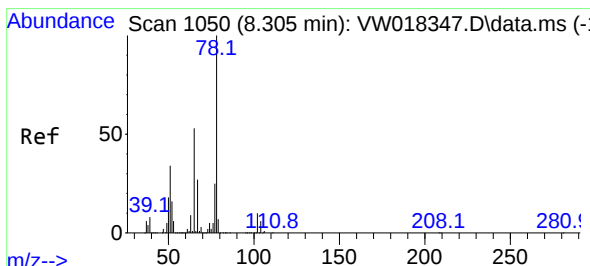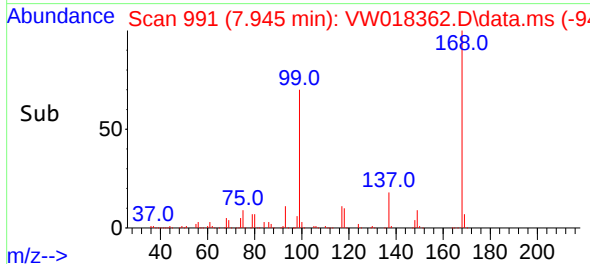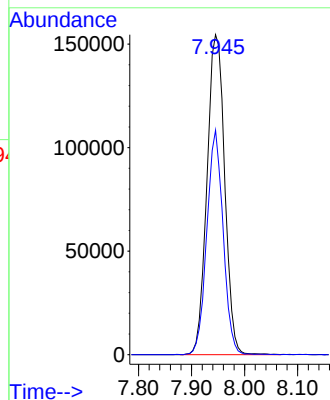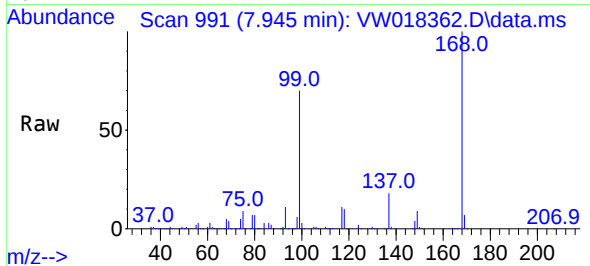

#33
1,2-Dichloroethane-d4
Concen: 51.64 ug/l
RT: 8.305 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36


Tgt Ion: 65 Resp: 197630
Ion Ratio Lower Upper
65 100
67 49.5 0.0 96.6

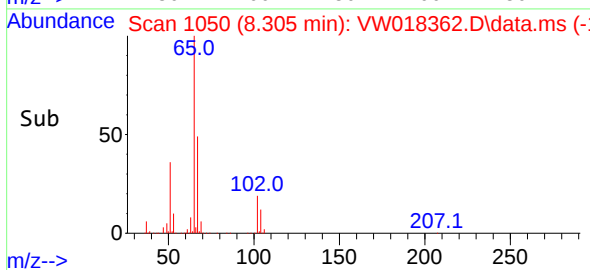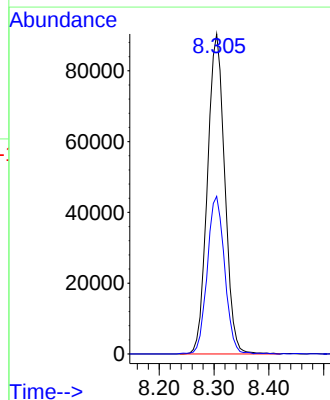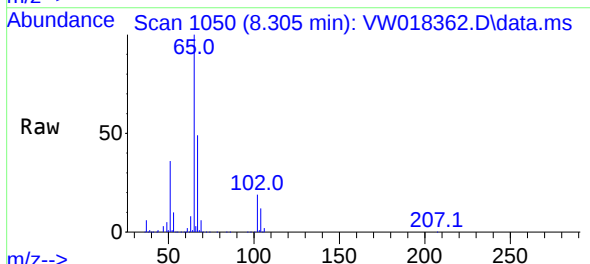



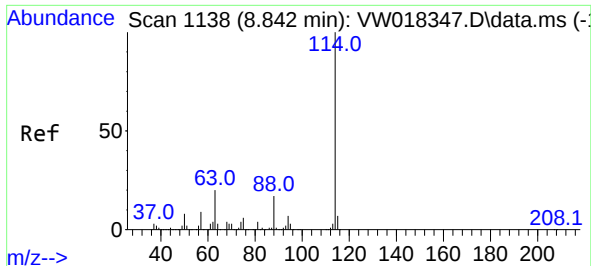


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.841 min Scan# 1138
Delta R.T. -0.001 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36


Instrument :
MSVOA_W
ClientSampleId :
VD0318SBL01

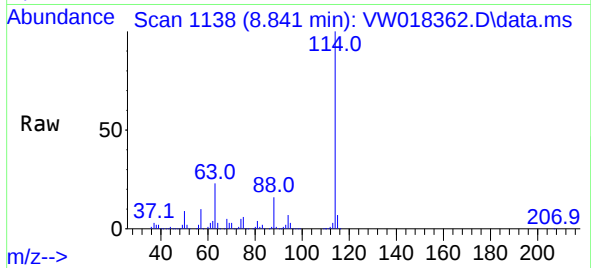



Tgt Ion:114 Resp: 586162
Ion Ratio Lower Upper
114 100
63 22.8 0.0 40.4
88 16.2 0.0 32.0

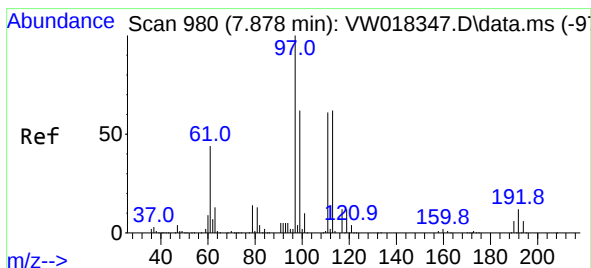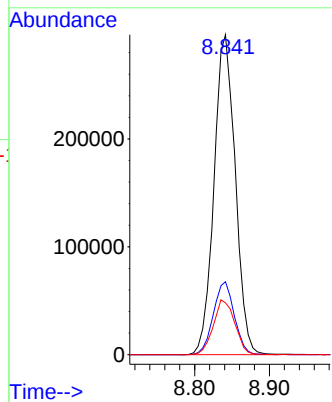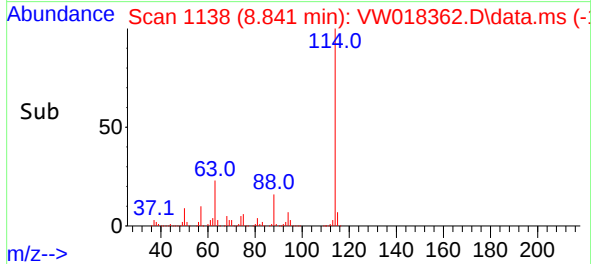


#35
Dibromofluoromethane
Concen: 50.30 ug/l
RT: 7.884 min Scan# 981
Delta R.T. 0.006 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36

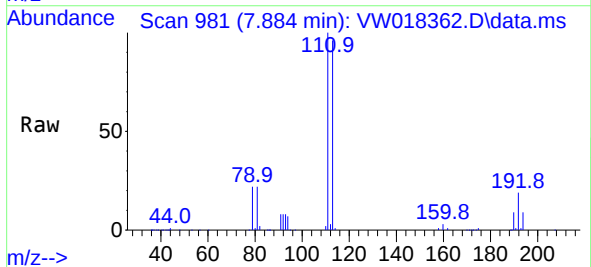

Tgt Ion:113 Resp: 171826
Ion Ratio Lower Upper
113 100
111 104.0 83.6 125.4
192 18.3 13.8 20.8



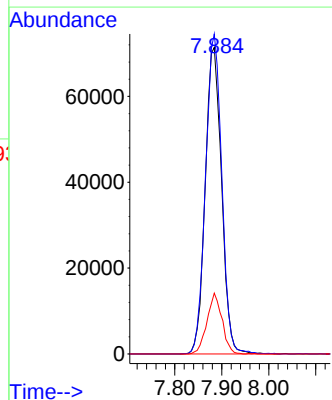
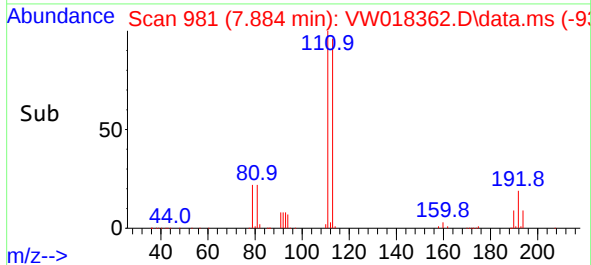


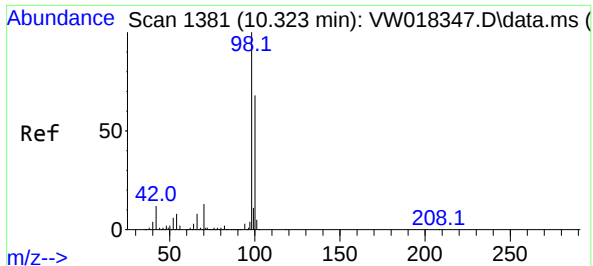

#50
Toluene-d8
Concen: 51.24 ug/l
RT: 10.323 min Scan# 1381
Delta R.T. -0.000 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36




Instrument :
MSVOA_W
ClientSampleId :
VD0318SBL01


Tgt Ion: 98 Resp: 696090
Ion Ratio Lower Upper
98 100
100 61.6 51.8 77.8

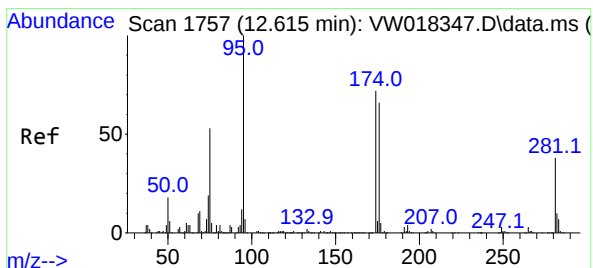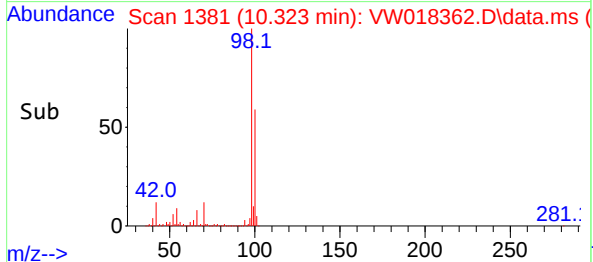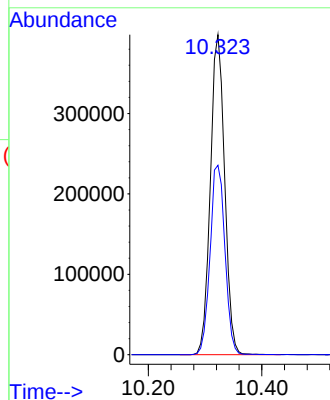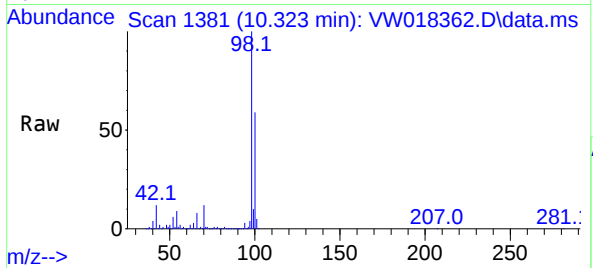

#62
4-Bromofluorobenzene
Concen: 48.73 ug/l
RT: 12.615 min Scan# 1757
Delta R.T. -0.000 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36

Tgt Ion: 95 Resp: 251278
Ion Ratio Lower Upper
95 100
174 67.7 0.0 132.8
176 67.1 0.0 131.4


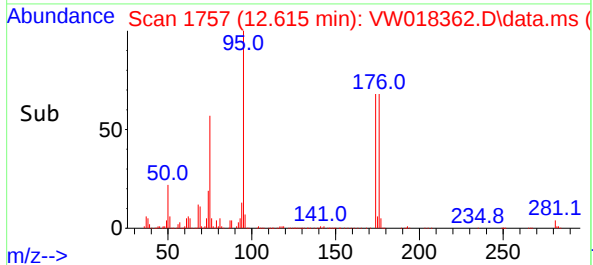
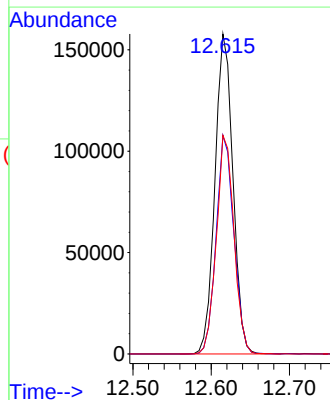
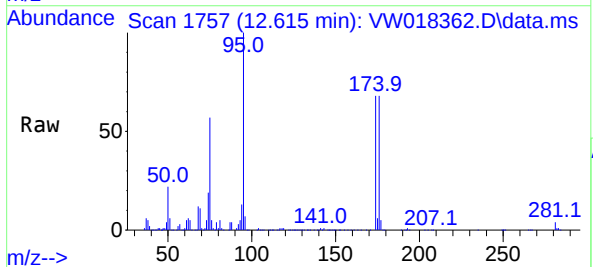


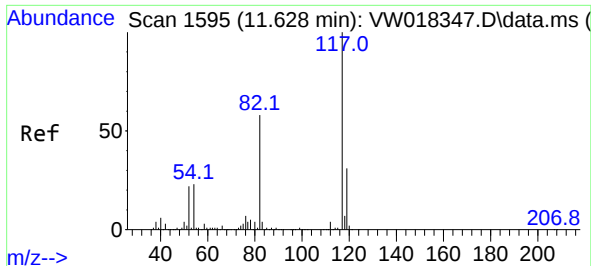

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.633 min Scan# 1596
Delta R.T. 0.005 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36

Instrument :
MSVOA_W
ClientSampleId :
VD0318SBL01

Tgt Ion:	117	Resp:	540682
Ion	Ratio	Lower	Upper
117	100		
82	58.2	43.1	64.7
119	33.2	25.1	37.7

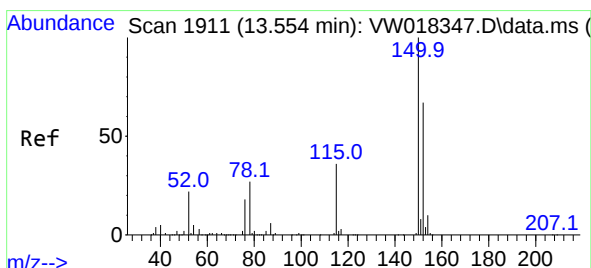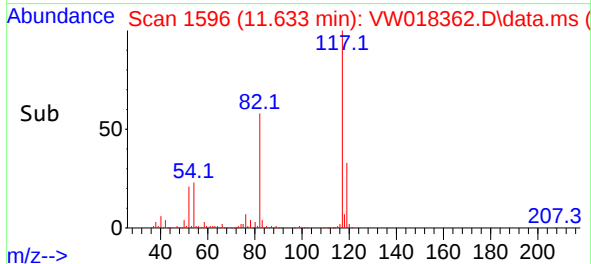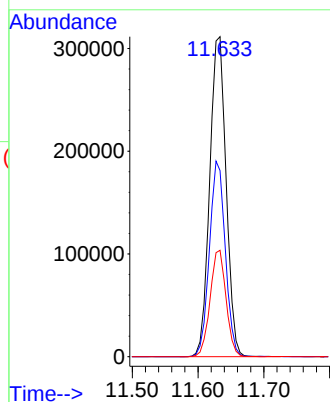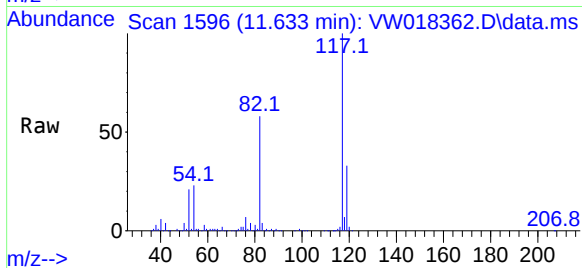

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.554 min Scan# 1911
Delta R.T. -0.000 min
Lab File: VW018362.D
Acq: 18 Mar 2021 10:36

Tgt Ion:	152	Resp:	248318
Ion	Ratio	Lower	Upper
152	100		
115	65.9	31.9	95.7
150	163.6	0.0	347.2

