
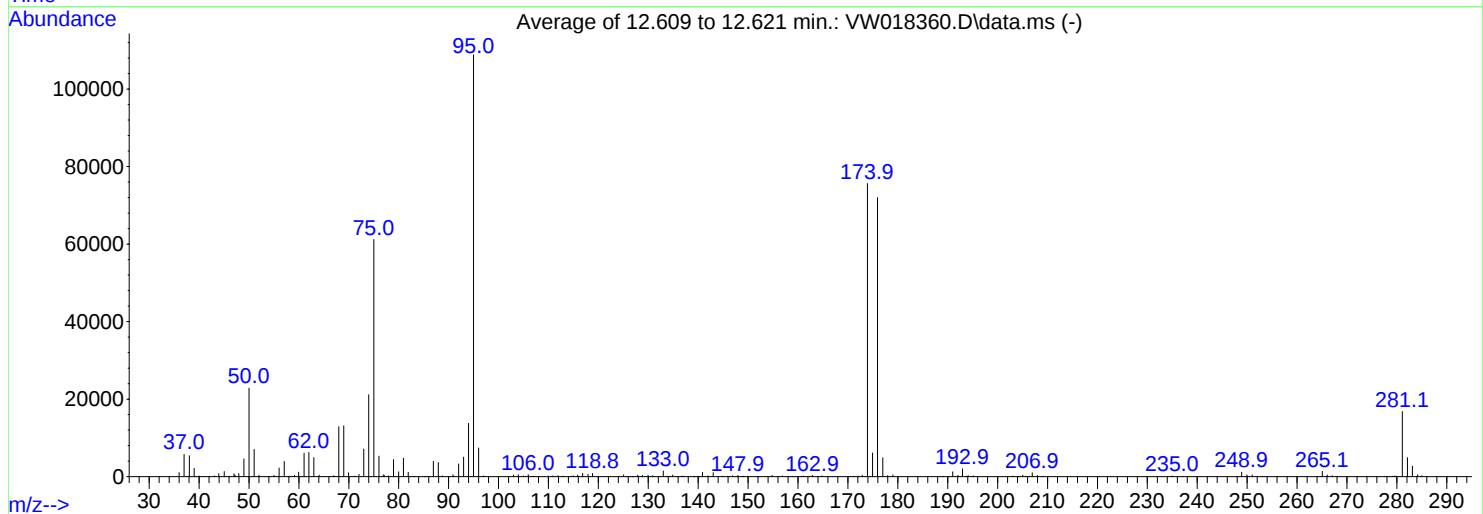


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031821\
 Data File : VW018360.D
 Acq On : 18 Mar 2021 08:42
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W031721S.M
 Title : SW846 8260
 Last Update : Wed Mar 17 18:51:14 2021

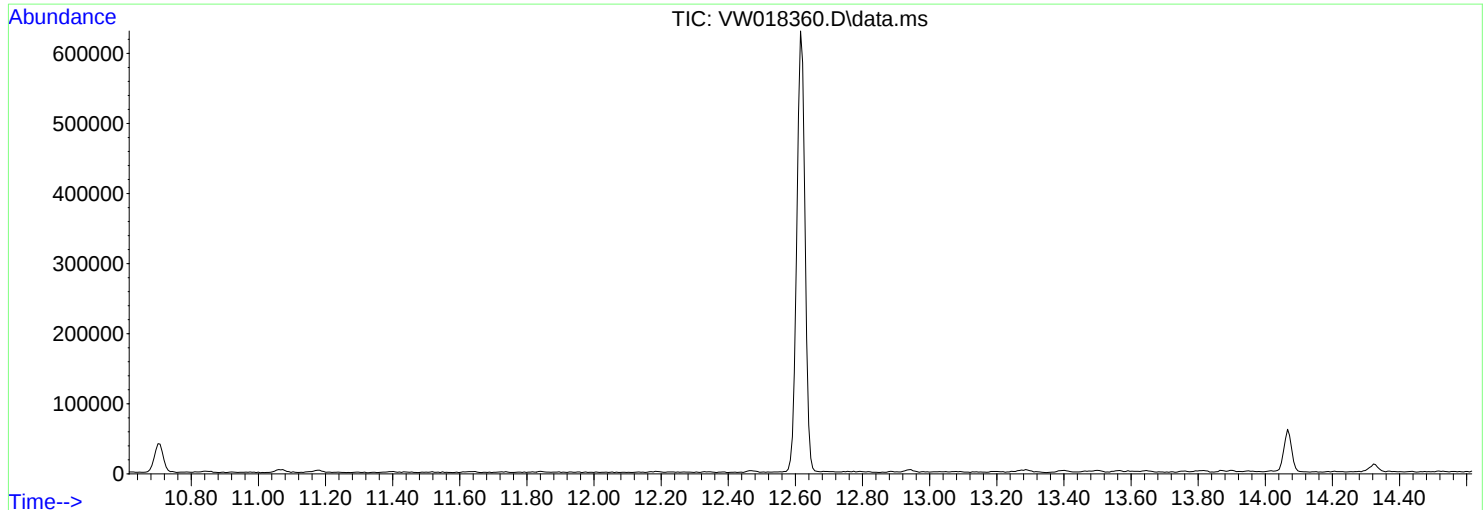

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	22843	PASS
75	95	30	60	56.2	61189	PASS
95	95	100	100	100.0	108829	PASS
96	95	5	9	6.8	7372	PASS
173	174	0.00	2	0.5	370	PASS
174	95	50	100	69.5	75624	PASS
175	174	5	9	8.1	6092	PASS
176	174	95	101	95.2	71987	PASS
177	176	5	9	6.7	4859	PASS