


Dichlorodifluoromethane

Response Ratio

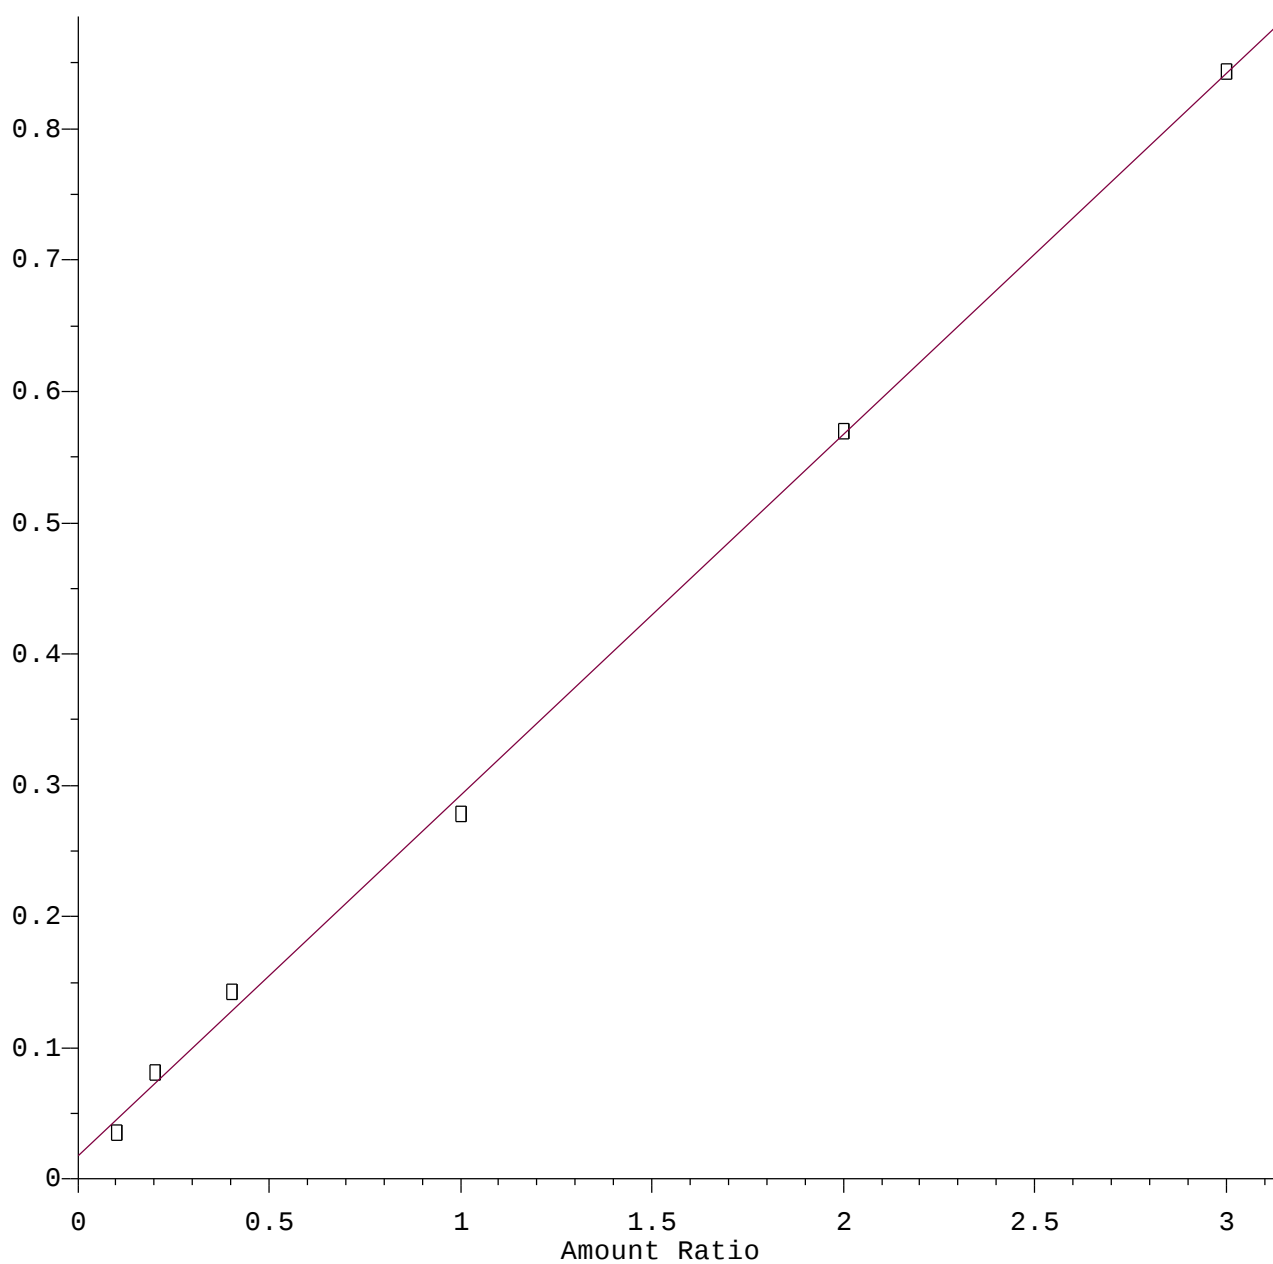


Resp Ratio = $2.75 \times 10^{-1} \times \text{Amt} + 1.83 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W031919S.M
Calibration Table Last Updated: Wed Mar 20 07:22:50 2019

Methylene Chloride

Response Ratio

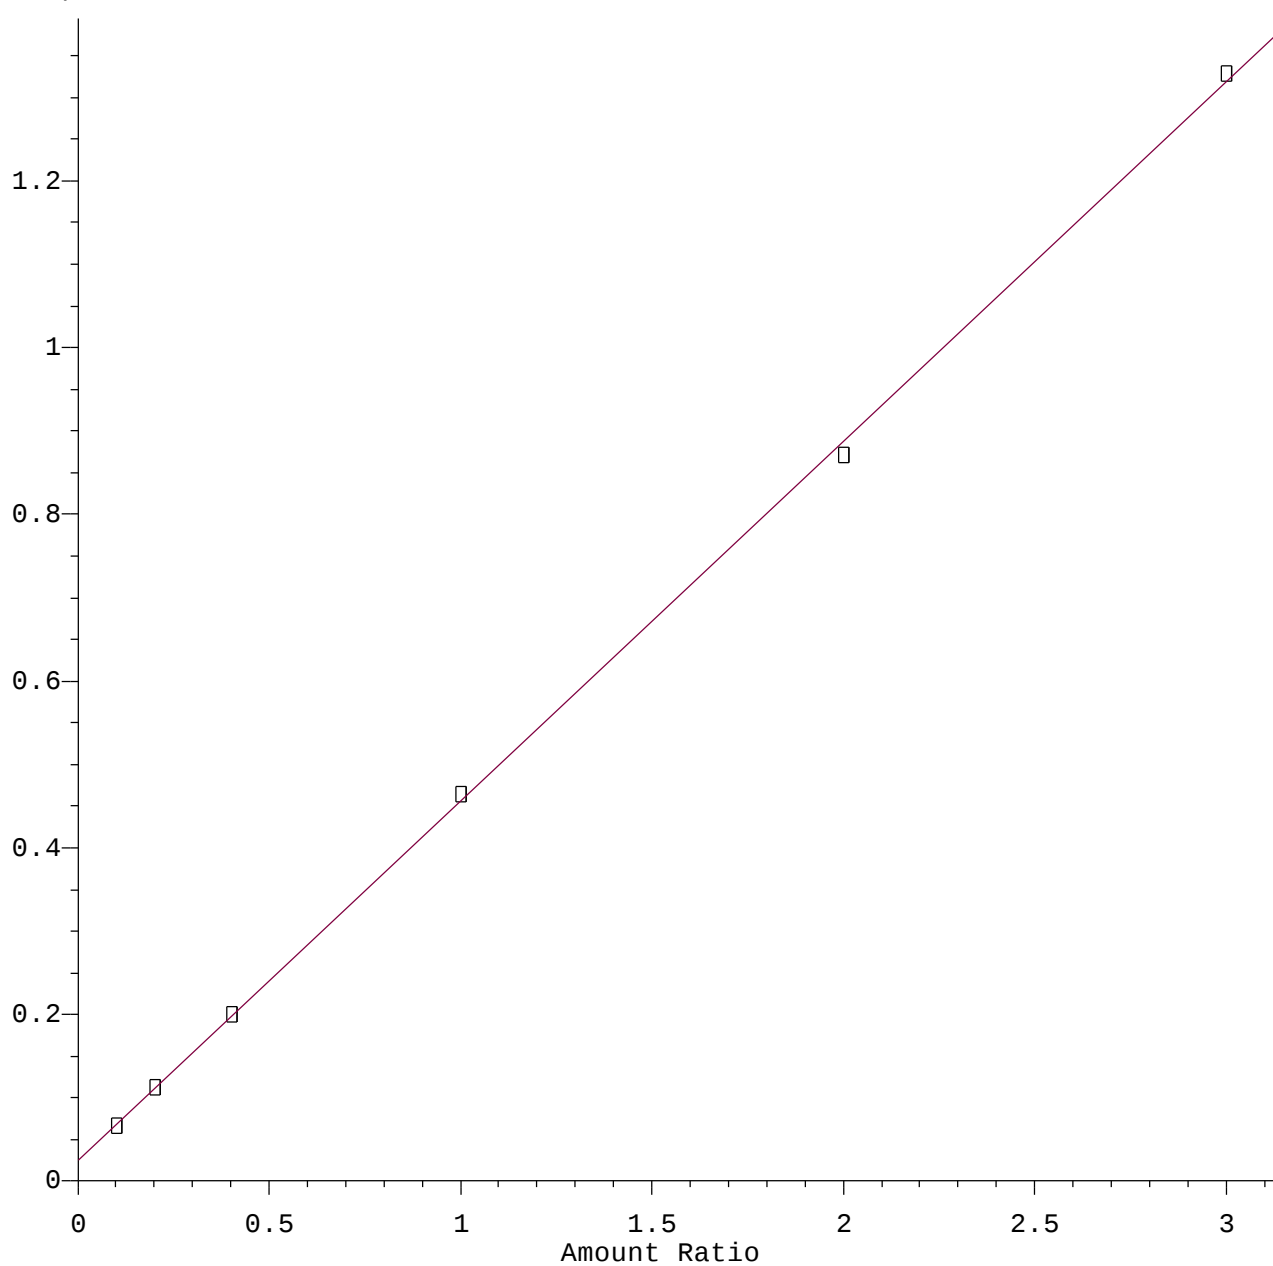

Resp Ratio = $4.32 \times 10^{-1} \times \text{Amt} + 2.45 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W031919S.M
Calibration Table Last Updated: Wed Mar 20 07:22:50 2019