


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW031919\
 Data File : VW009232.D
 Acq On : 19 Mar 2019 09:50
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W031919S.M
 Title : SW846 8260
 Last Update : Wed Mar 20 07:22:50 2019

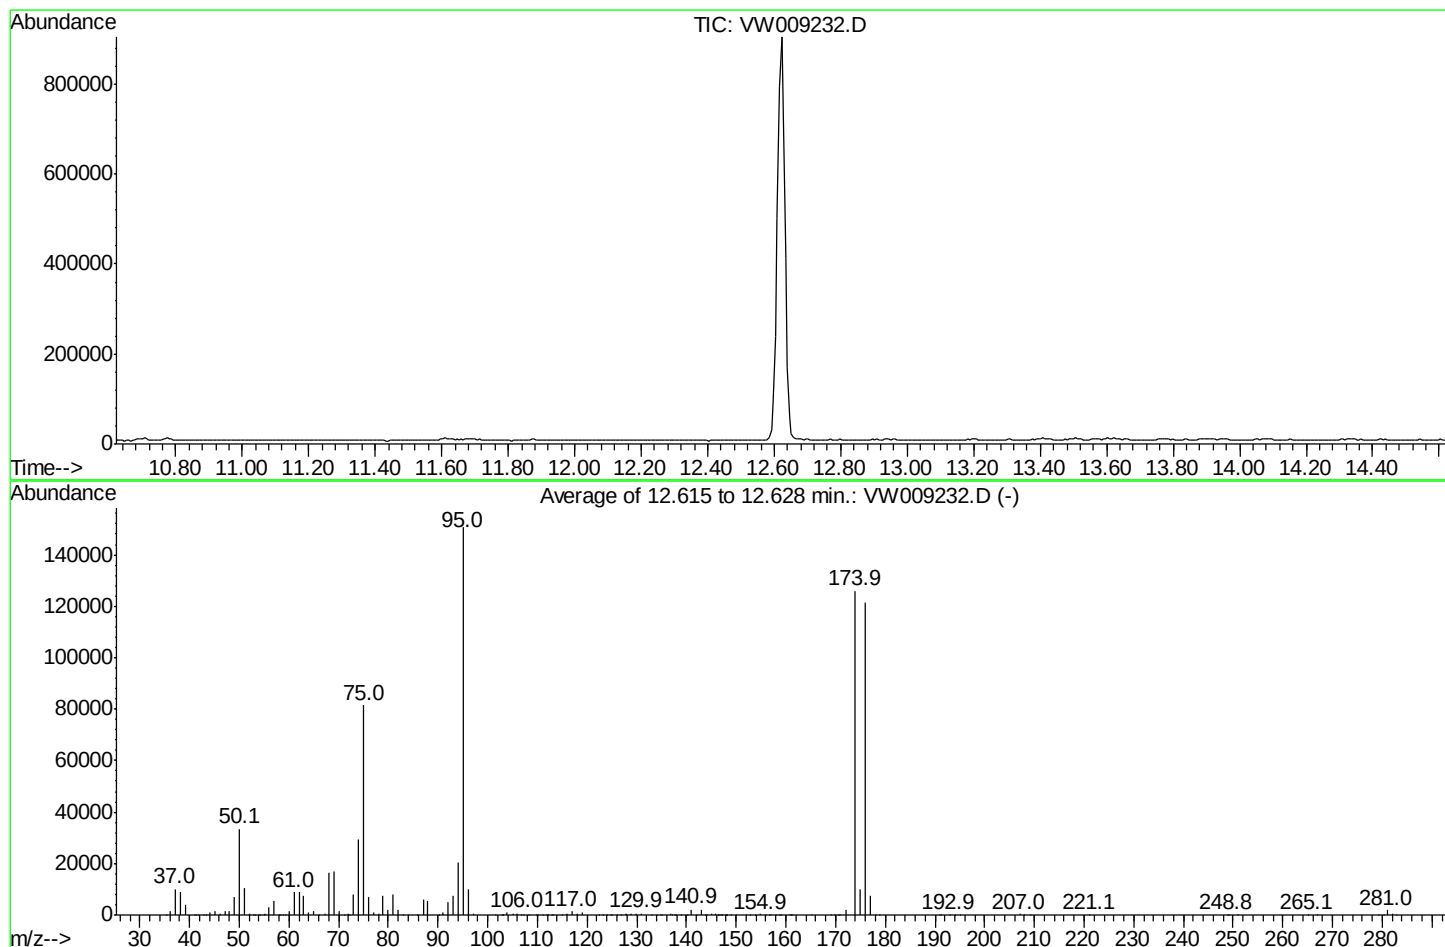

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	33469	PASS
75	95	30	60	54.0	81373	PASS
95	95	100	100	100.0	150634	PASS
96	95	5	9	6.5	9795	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.7	126021	PASS
175	174	5	9	8.0	10086	PASS
176	174	95	101	96.1	121154	PASS
177	176	5	9	6.2	7516	PASS