


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
Data File : VW018379.D
Acq On : 19 Mar 2021 11:17
Operator : SY/VA
Sample : M1685-02
Misc : 5.65G/10ML/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG488

Manual Integrations
APPROVED

MMDadoda
3/22/2021 4:13:52 PM

Quant Time: Mar 20 01:38:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 20 01:36:44 2021
Response via : Initial Calibration

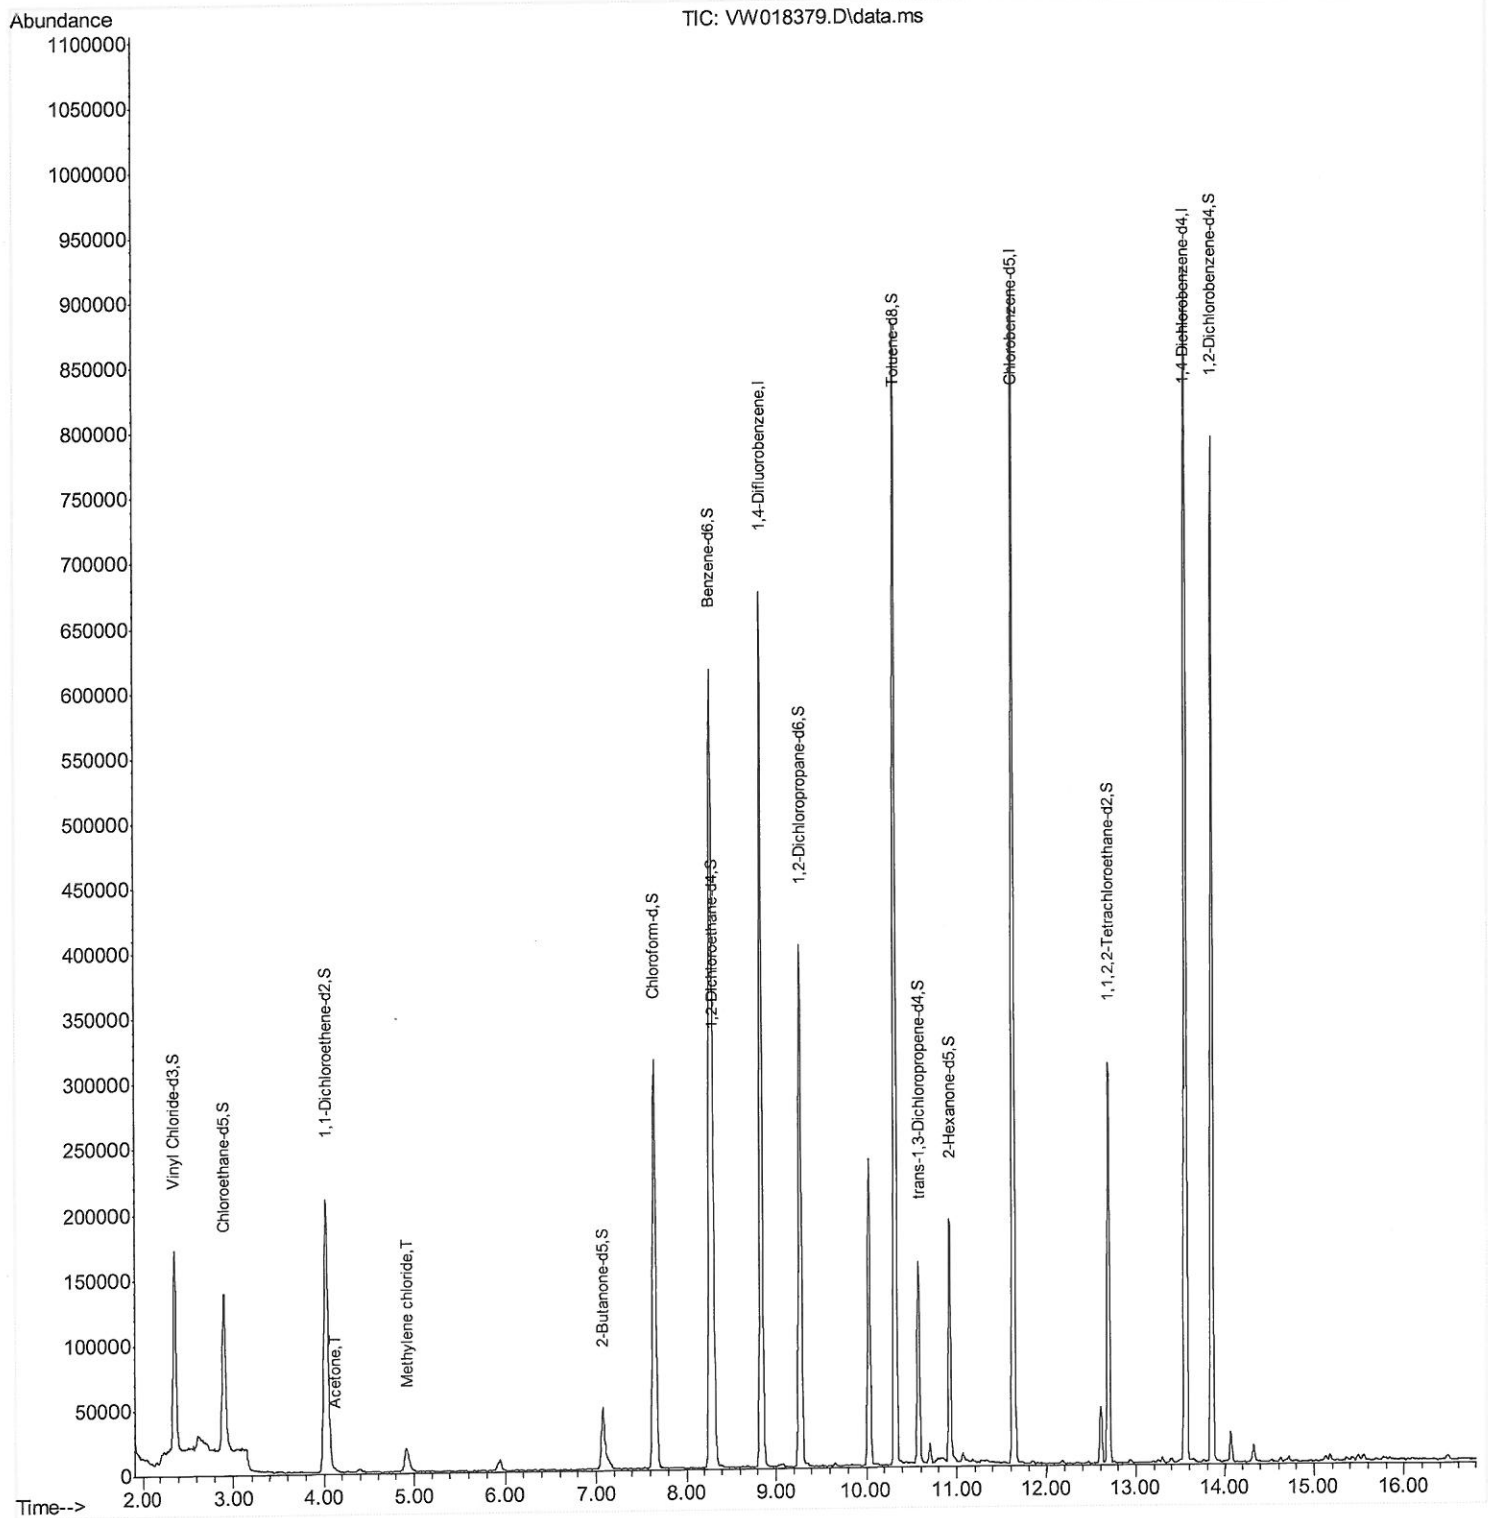

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
 Data File : VW018379.D
 Acq On : 19 Mar 2021 11:17
 Operator : SY/VA
 Sample : M1685-02
 Misc : 5.65G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG488

Manual Integrations
 APPROVED

MMDadoda
 3/22/2021 4:13:52 PM

Quant Time: Mar 20 01:38:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 01:36:44 2021
 Response via : Initial Calibration

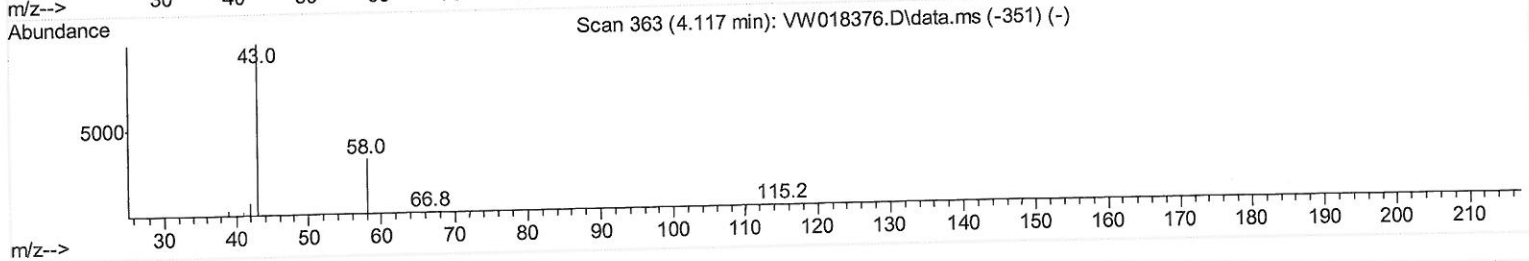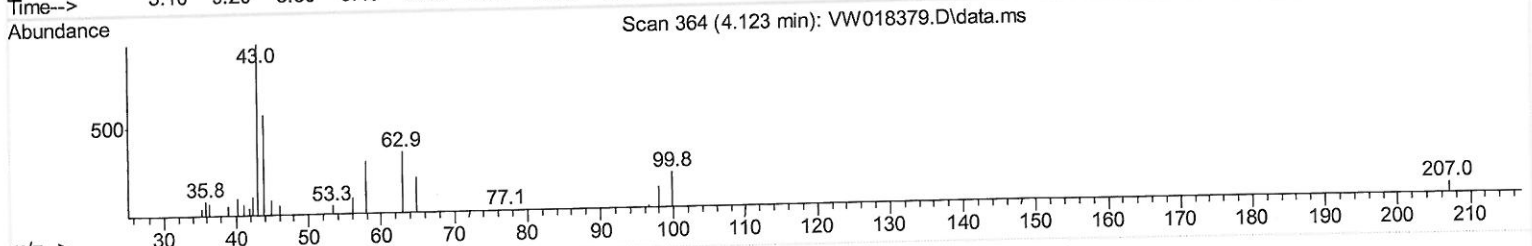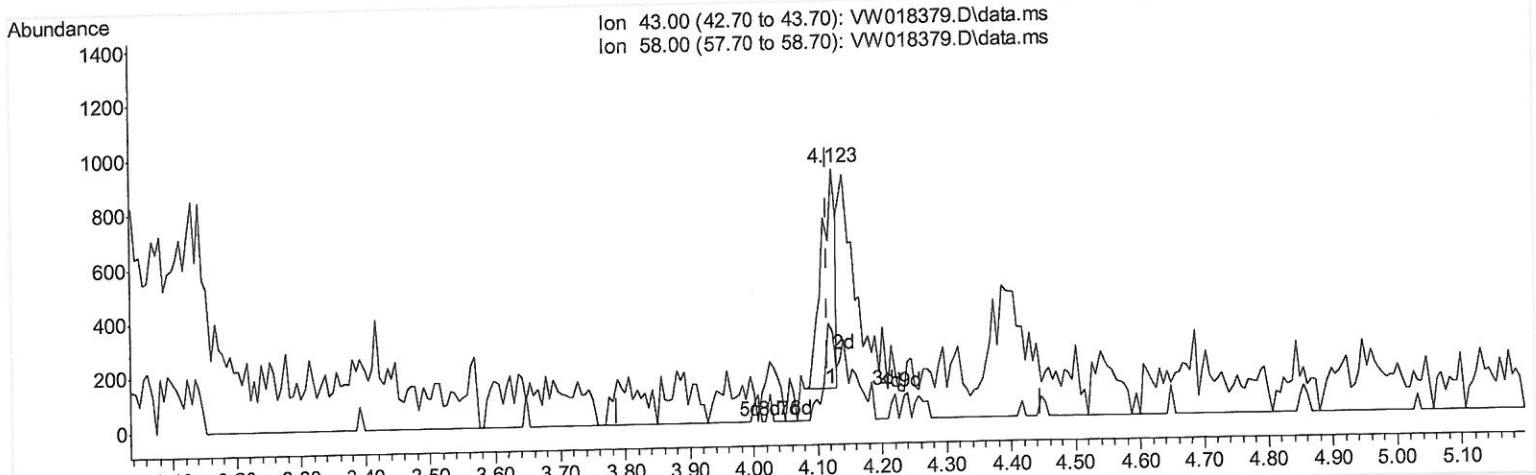

TIC: VW018379.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 1.03 ug/L

response 1217

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	29.91
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
 Data File : VW018379.D
 Acq On : 19 Mar 2021 11:17
 Operator : SY/VA
 Sample : M1685-02
 Misc : 5.65G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG488

Manual Integrations
 APPROVED

MMDadoda
 3/22/2021 4:13:52 PM

Quant Time: Mar 20 01:38:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 01:36:44 2021
 Response via : Initial Calibration

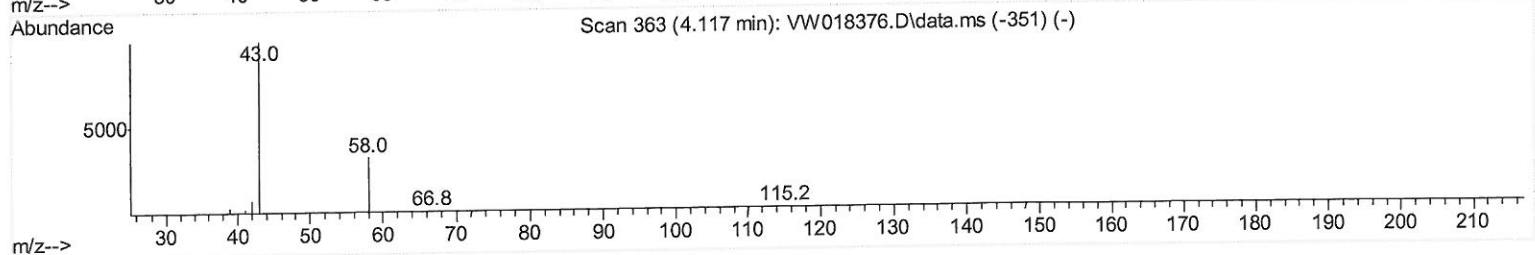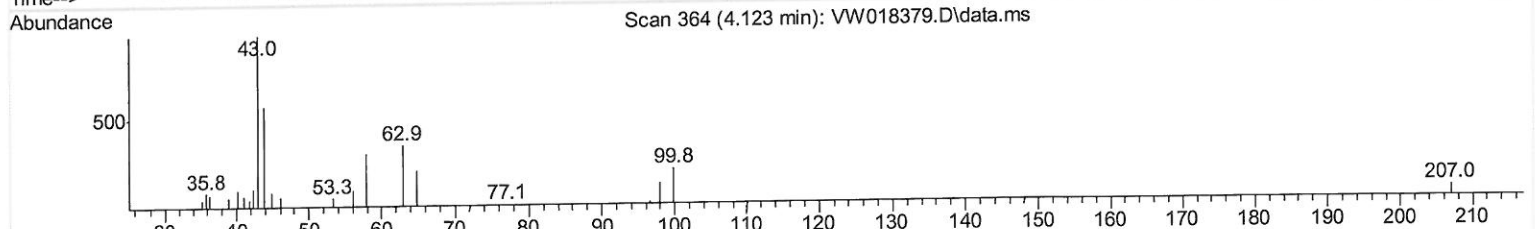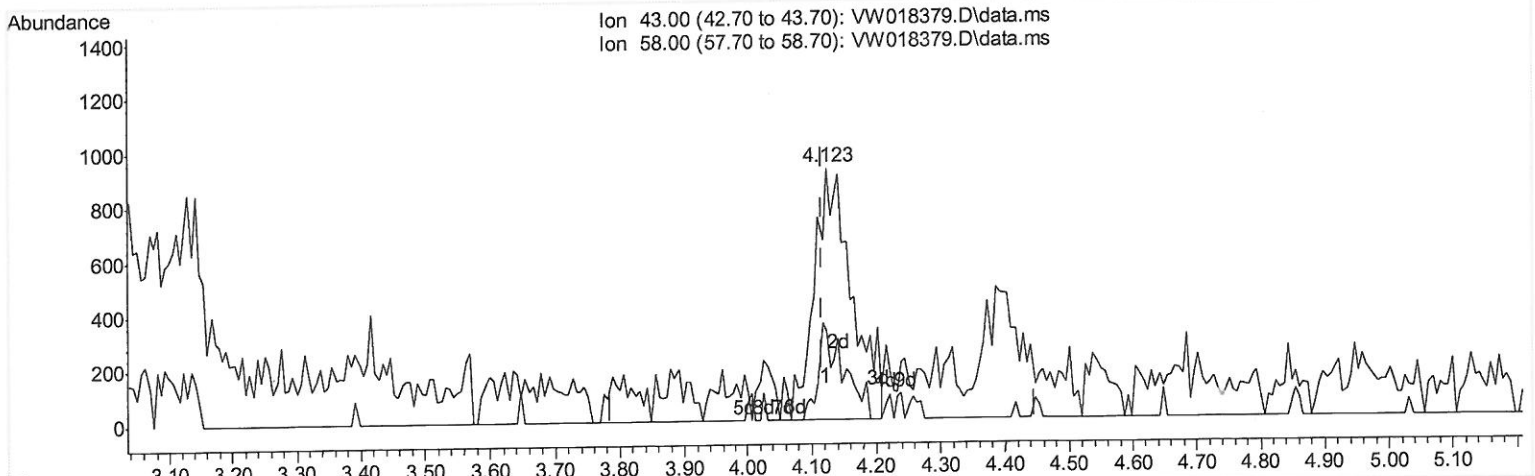

TIC: VW018379.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.13 ug/L m

response 3715

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	9.80
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
 3/20/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
 Data File : VW018379.D
 Acq On : 19 Mar 2021 11:17
 Operator : SY/VA
 Sample : M1685-02
 Misc : 5.65G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG488

Manual Integrations
 APPROVED

MMDadoda
 3/22/2021 4:13:52 PM

Quant Time: Mar 20 01:38:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 01:36:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	532683	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	486179	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	226970	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	191982	25.90	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.60%			
7) Chloroethane-d5	2.898	69	167999	25.89	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.56%			
10) 1,1-Dichloroethene-d2	4.019	63	234904	18.35	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 73.40%			
20) 2-Butanone-d5	7.080	46	78012	47.27	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 94.54%			
24) Chloroform-d	7.647	84	306112	22.56	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 90.24%			
26) 1,2-Dichloroethane-d4	8.305	65	183451	23.16	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 92.64%			
29) Benzene-d6	8.275	84	608980	23.56	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 94.24%			
33) 1,2-Dichloropropane-d6	9.275	67	173218	23.23	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 92.92%			
37) Toluene-d8	10.323	98	577220	23.19	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 92.76%			
38) trans-1,3-Dichloroprop...	10.579	79	82553	21.47	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 85.88%			
39) 2-Hexanone-d5	10.921	63	65490	44.89	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 89.78%			
48) 1,1,2,2-Tetrachloroeth...	12.689	84	149109	22.36	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 89.44%			
61) 1,2-Dichlorobenzene-d4	13.853	152	185956	23.05	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 92.20%			
Target Compounds						
13) Acetone	4.123	43	3715m	3.13	ug/L	Qvalue
16) Methylene chloride	4.922	84	15194	1.74	ug/L	93

2 MD
 3/30/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed