


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
Data File : VW018403.D
Acq On : 19 Mar 2021 22:03
Operator : SY/VA
Sample : M1698-16
Misc : 5.78G/10ML/MSVOA_W/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4L4

Manual Integrations
APPROVED

MMDadoda
3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
Qlast Update : Sat Mar 20 03:58:53 2021
Response via : Initial Calibration

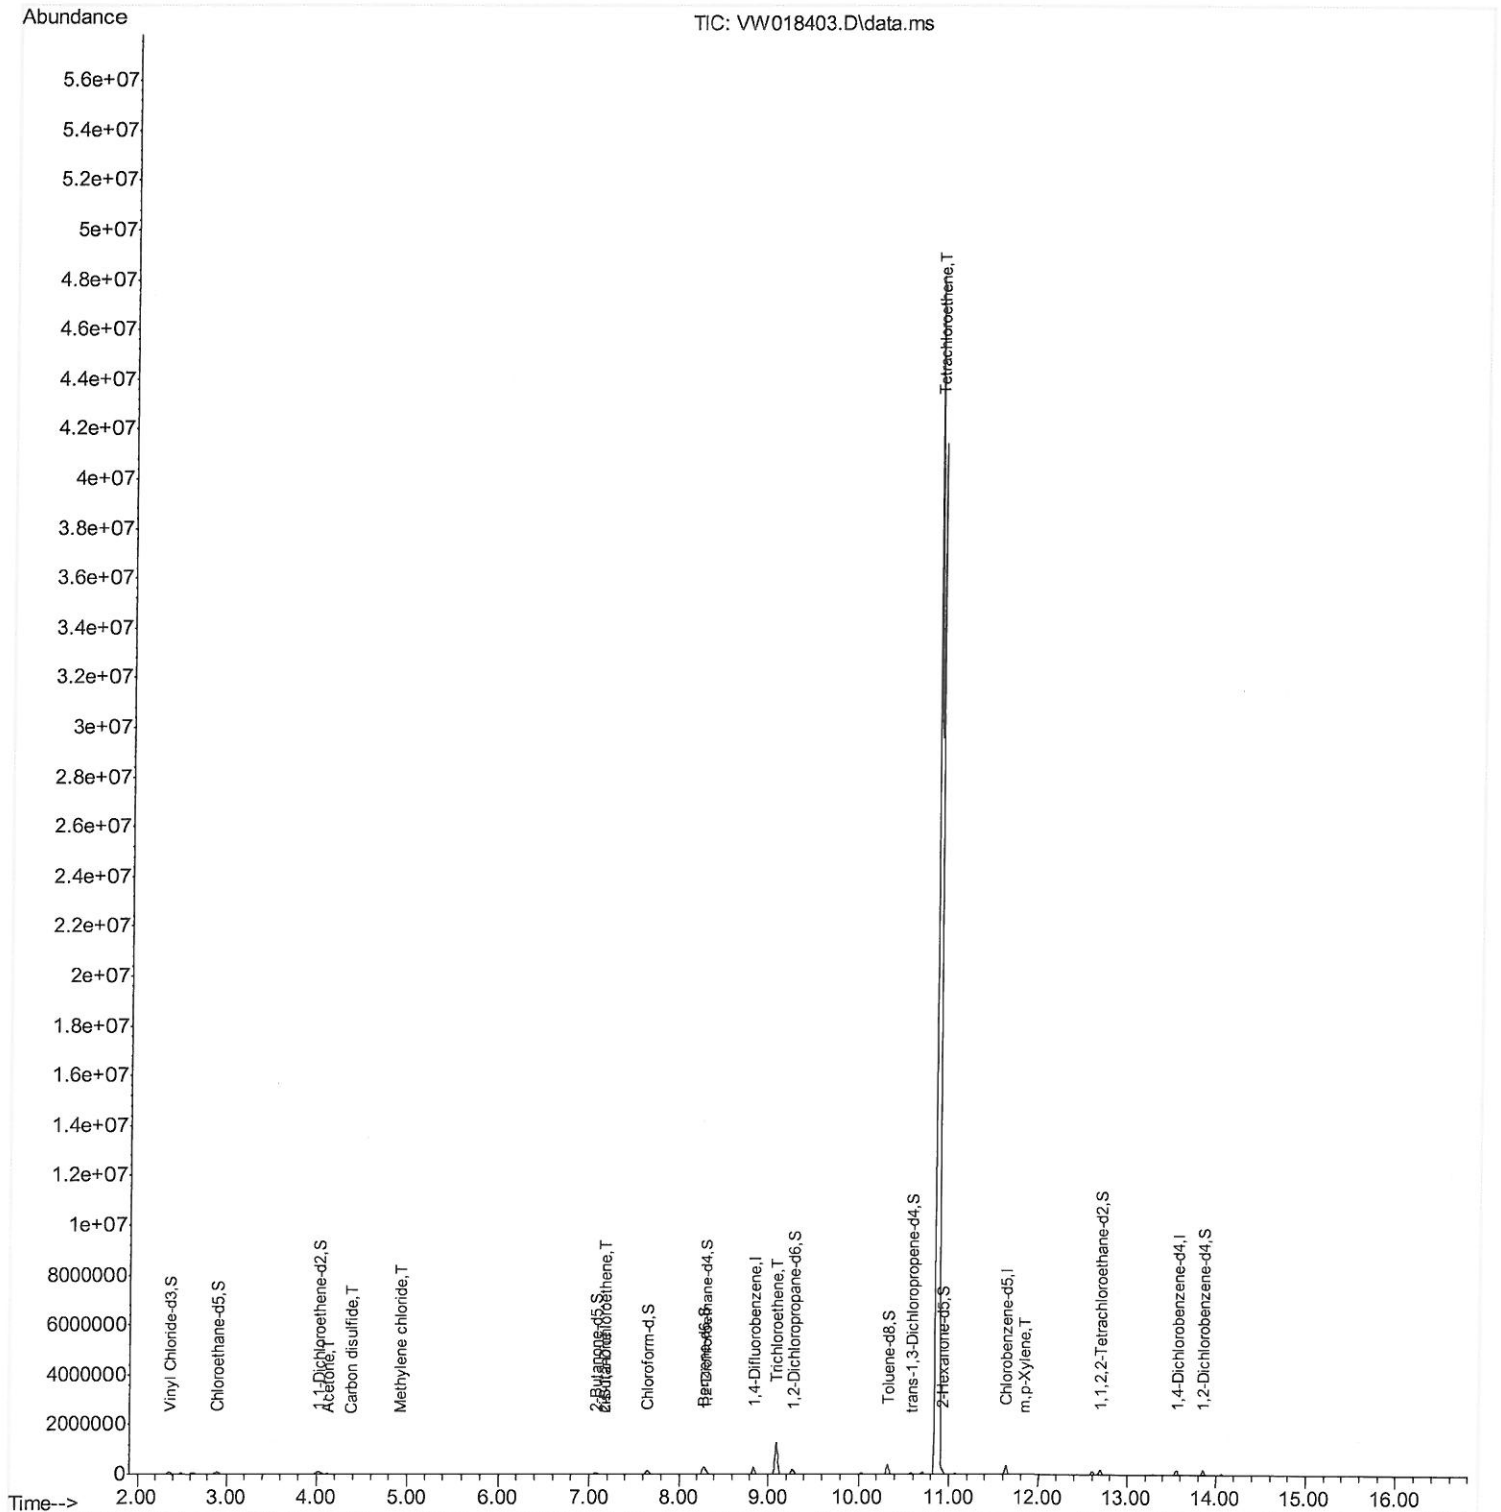

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
 Data File : VW018403.D
 Acq On : 19 Mar 2021 22:03
 Operator : SY/VA
 Sample : M1698-16
 Misc : 5.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4L4

Manual Integrations
 APPROVED

MMDadoda
 3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 03:58:53 2021
 Response via : Initial Calibration

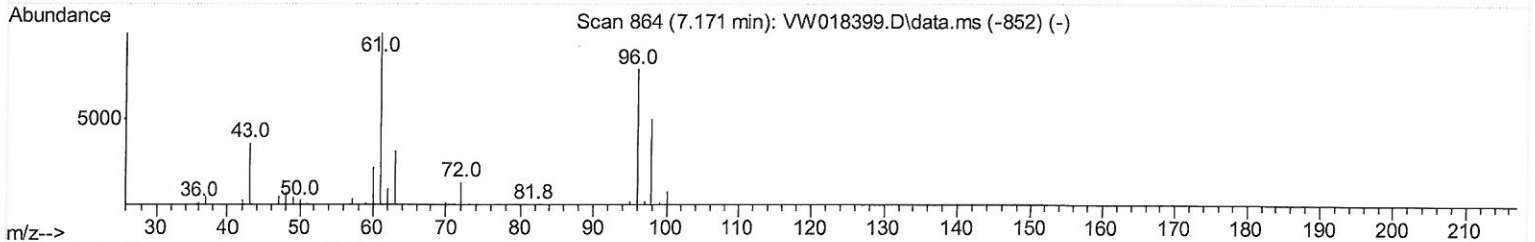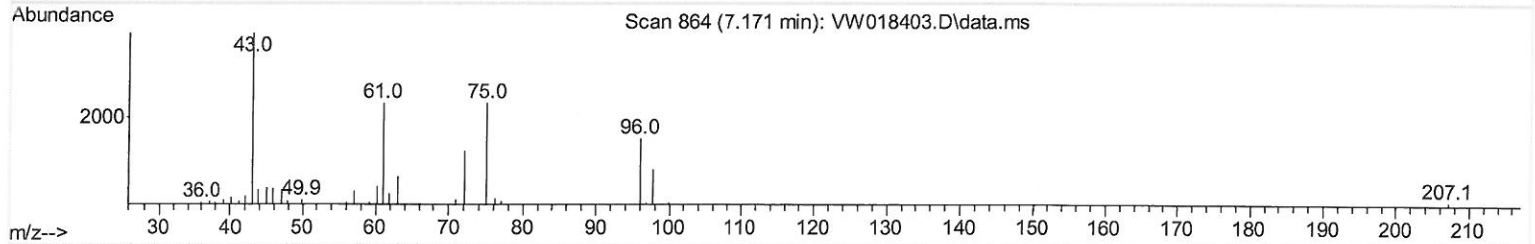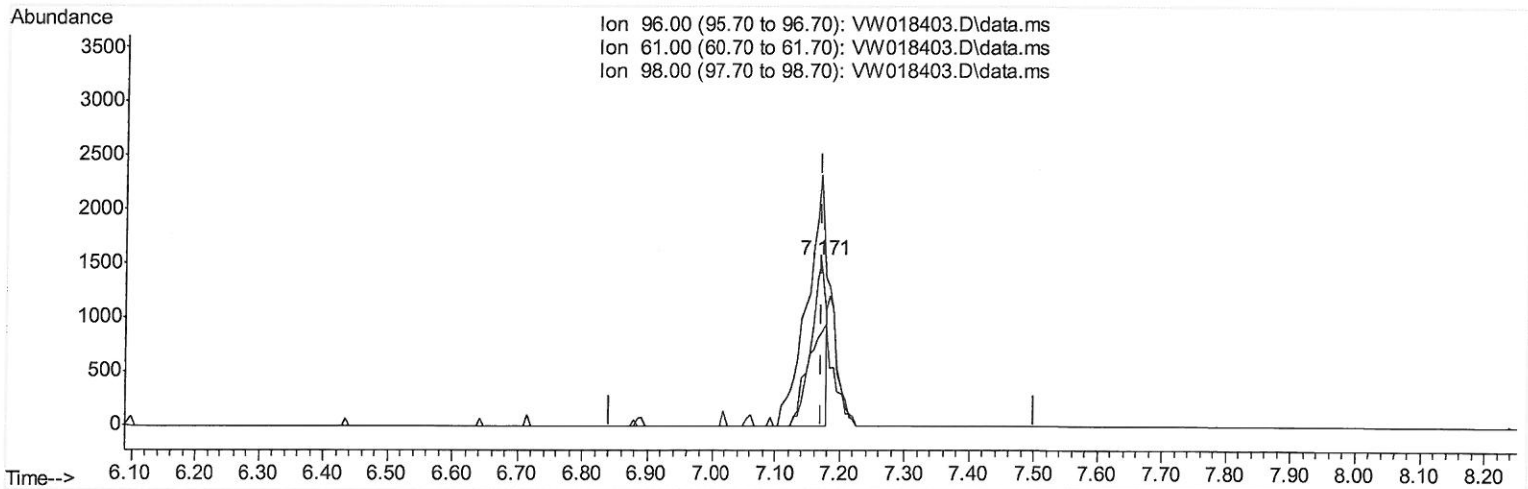

TIC: VW018403.D\data.ms

(22) cis-1,2-Dichloroethene (T)

7.171min (-0.000) 0.72 ug/L

response 2450

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	121.20	151.79
98.00	64.50	55.45
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
Data File : VW018403.D
Acq On : 19 Mar 2021 22:03
Operator : SY/VA
Sample : M1698-16
Misc : 5.78G/10ML/MSVOA_W/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4L4

Manual Integrations
APPROVED

MMDadoda
3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 20 03:58:53 2021
Response via : Initial Calibration

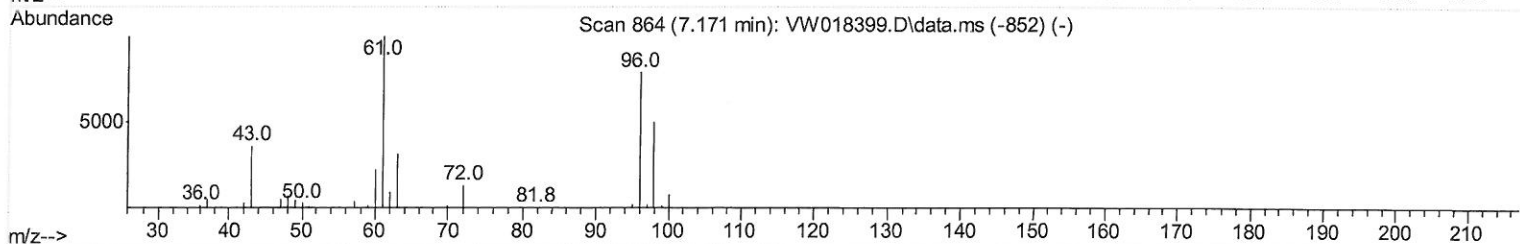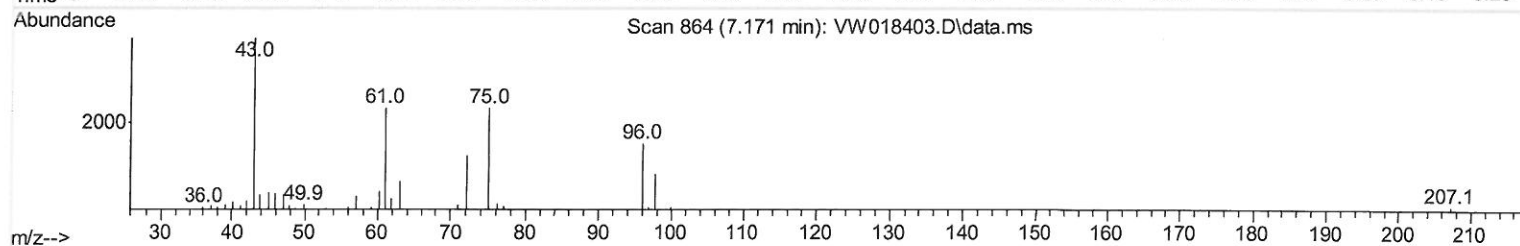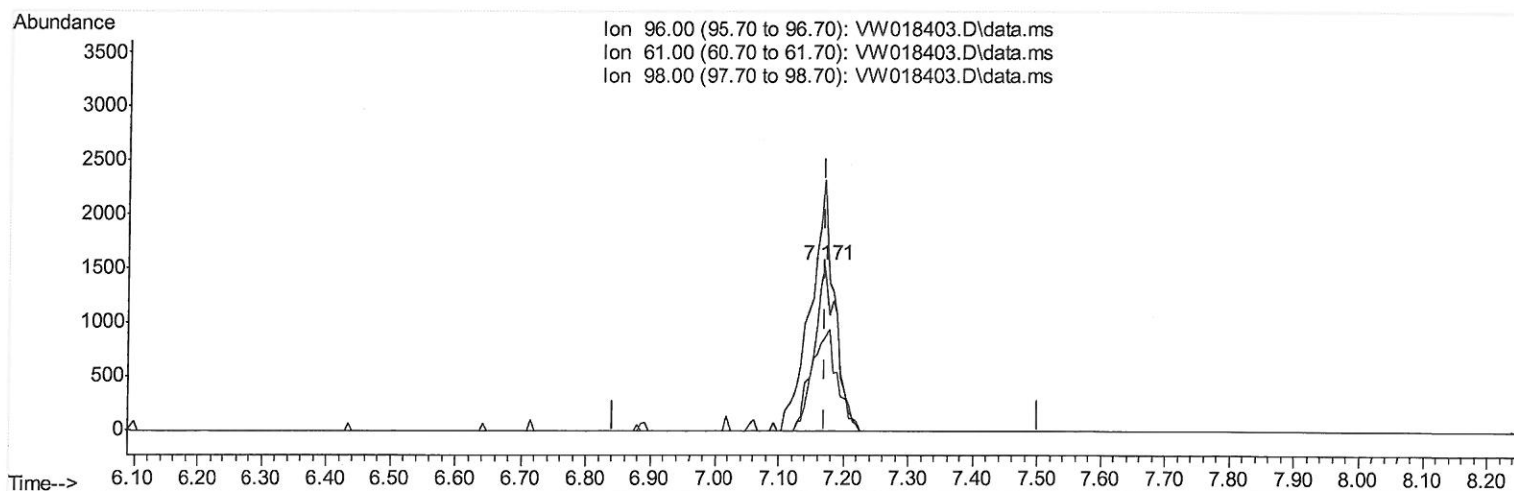

TIC: VW018403.D\data.ms

(22) cis-1,2-Dichloroethene (T)

7.171min (-0.000) 1.10 ug/L m

response 3721

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	121.20	151.79
98.00	64.50	55.45
0.00	0.00	0.00

MD
3/30/21

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
Data File : VW018403.D
Acq On : 19 Mar 2021 22:03
Operator : SY/VA
Sample : M1698-16
Misc : 5.78G/10ML/MSVOA_W/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG4L4

Manual Integrations
APPROVED

MMDadoda
3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 20 03:58:53 2021
Response via : Initial Calibration

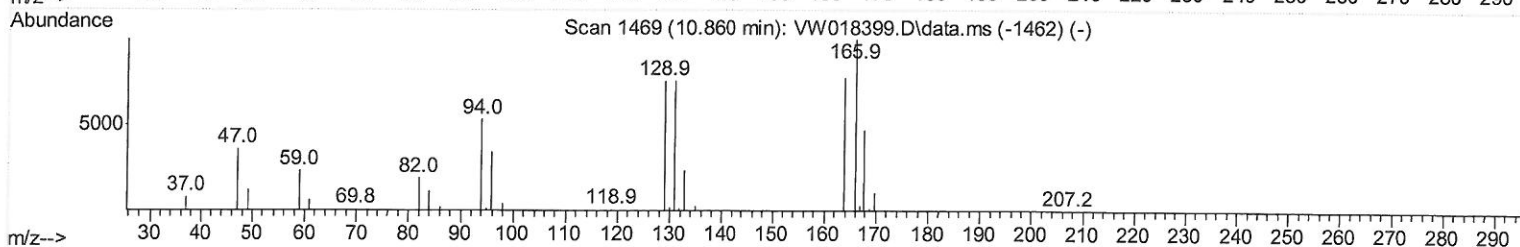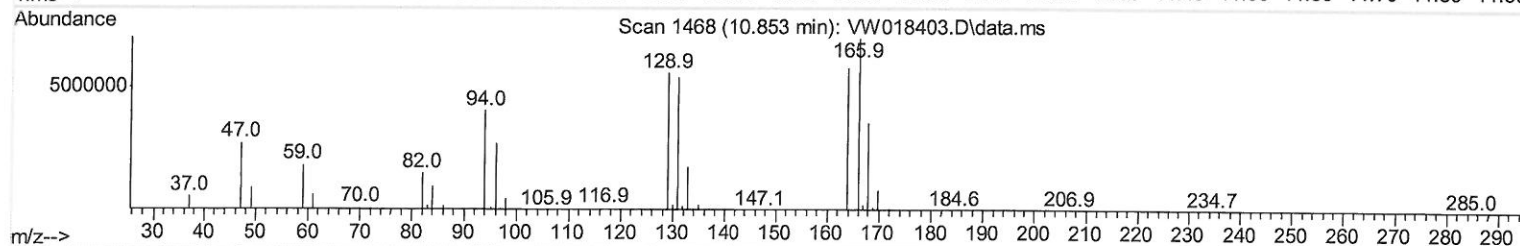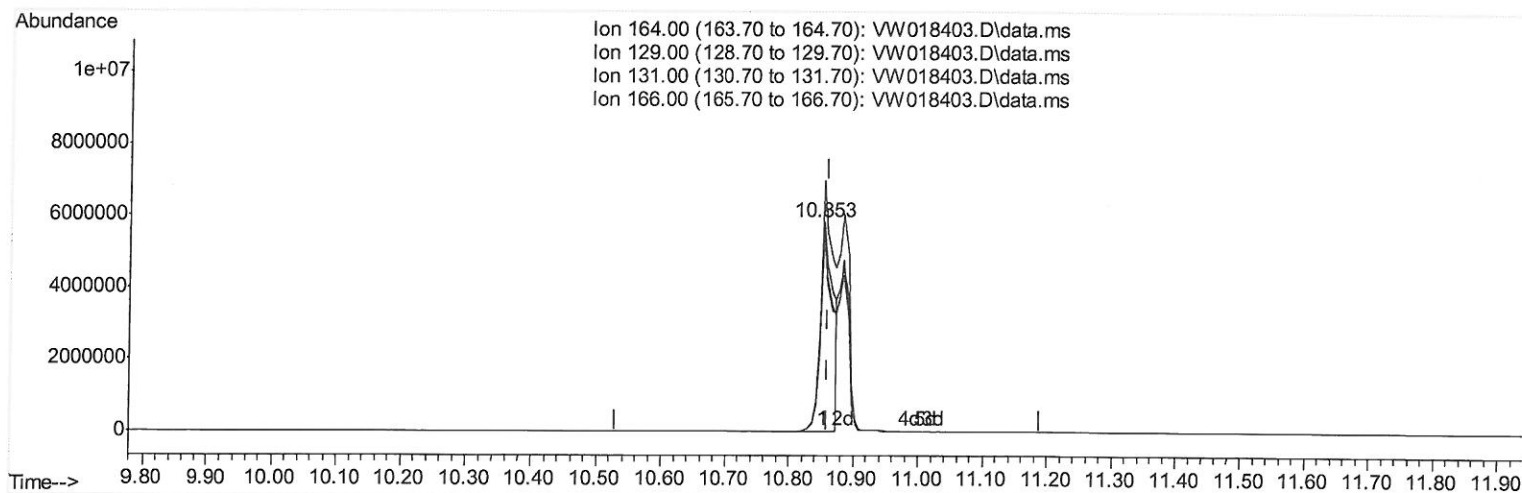

TIC: VW018403.D\data.ms

(47) Tetrachloroethene (T)

10.853min (-0.006) 3762.99 ug/L

response 7722927

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	98.30	96.11
131.00	97.50	93.13
166.00	136.30	120.28

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
Data File : VW018403.D
Acq On : 19 Mar 2021 22:03
Operator : SY/VA
Sample : M1698-16
Misc : 5.78G/10ML/MSVOA_W/SOIL
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG4L4

Manual Integrations
APPROVED

MMDadoda
3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 20 03:58:53 2021
Response via : Initial Calibration

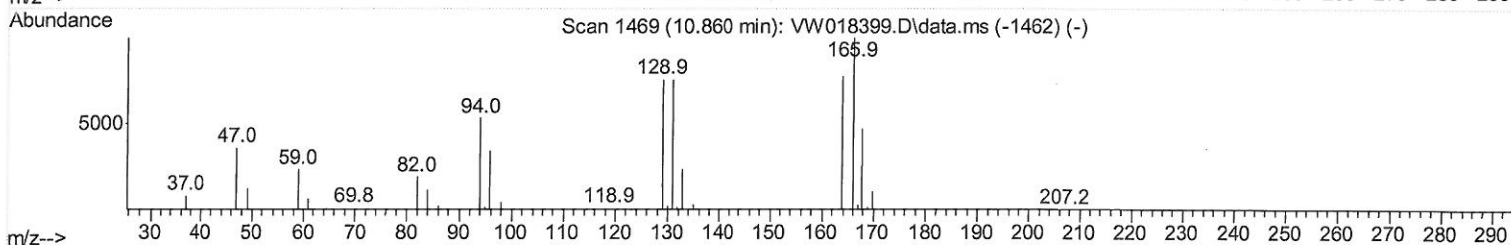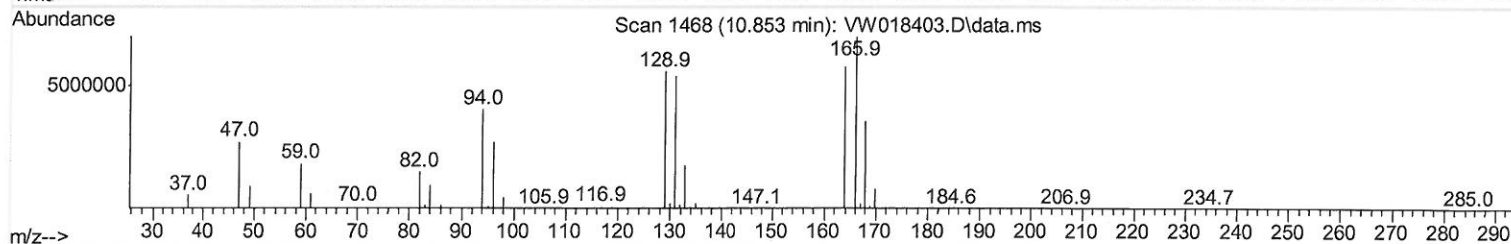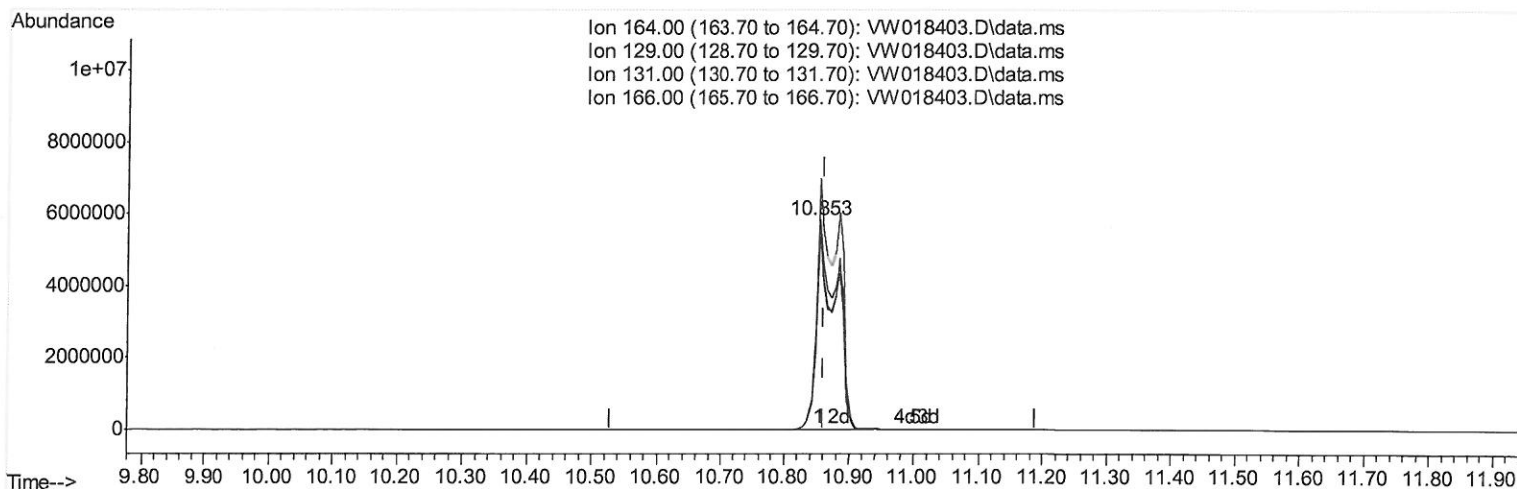

TIC: VW018403.D\data.ms

(47) Tetrachloroethene (T)

10.853min (-0.006) 6175.91 ug/L m

response 12675058

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	98.30	96.11
131.00	97.50	93.13
166.00	136.30	120.28

7 mg
3/30/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031921\
 Data File : VW018403.D
 Acq On : 19 Mar 2021 22:03
 Operator : SY/VA
 Sample : M1698-16
 Misc : 5.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4L4

Manual Integrations
 APPROVED

MMDadoda
 3/22/2021 4:14:34 PM

Quant Time: Mar 20 04:00:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 03:58:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	232781	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	168929	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	49805	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	97065	29.96	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	119.84%		
7) Chloroethane-d5	2.891	69	87814	30.97	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	123.88%		
10) 1,1-Dichloroethene-d2	4.025	63	116682	20.86	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	83.44%		
20) 2-Butanone-d5	7.074	46	89015	123.43	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	246.86%#		
24) Chloroform-d	7.647	84	152391	25.70	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	102.80%		
26) 1,2-Dichloroethane-d4	8.305	65	97977	28.31	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	113.24%		
29) Benzene-d6	8.275	84	295653	32.92	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	131.68%		
33) 1,2-Dichloropropane-d6	9.274	67	86806	33.51	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	134.04%#		
37) Toluene-d8	10.323	98	248411	28.73	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	114.92%		
38) trans-1,3-Dichloroprop...	10.579	79	21609	16.17	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	64.68%		
39) 2-Hexanone-d5	10.921	63	52009	102.59	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	205.18%#		
48) 1,1,2,2-Tetrachloroeth...	12.688	84	84099	36.29	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	145.16%#		
61) 1,2-Dichlorobenzene-d4	13.853	152	48257	27.25	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	109.00%		
Target Compounds						
13) Acetone	4.117	43	40240	77.67	ug/L	99
14) Carbon disulfide	4.385	76	5073	0.58	ug/L #	85
16) Methylene chloride	4.922	84	15614	4.09	ug/L	91
21) 2-Butanone	7.171	43	10533	12.80	ug/L	83
22) cis-1,2-Dichloroethene	7.171	96	3721m	1.10	ug/L	
35) Trichloroethene	9.092	95	430228	159.17	ug/L	99
47) Tetrachloroethene	10.853	164	12675058m	6175.91	ug/L	
54) m,p-Xylene	11.841	106	1213	0.25	ug/L	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 3/30/21