

Data File : VW009286.D
Acq On : 20 Mar 2019 14:42
Operator : SY/VA
Sample : K1986-08
Misc : 5.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0Z6

Quant Time: Mar 21 10:33:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	447716	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	423046	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	196158	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	140850	26.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.32%
7) Chloroethane-d5	2.89	69	132629	21.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.76%
10) 1,1-Dichloroethene-d2	4.01	63	220014	19.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.12%
20) 2-Butanone-d5	7.23	46	211	0.10	ug/L	0.15
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.20%#
24) Chloroform-d	7.64	84	298069	24.40	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	8.30	65	176285	23.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.80%
29) Benzene-d6	8.27	84	574389	24.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.48%
33) 1,2-Dichloropropane-d6	9.27	67	173132	24.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.84%
37) Toluene-d8	10.32	98	522706	24.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.92%
38) trans-1,3-Dichloropropene-	10.58	79	75797	21.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.16%
39) 2-Hexanone-d5	10.93	63	67842	39.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.94%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	146792	21.27	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	193735	25.76	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.04%


Target Compounds					Qvalue
42) cis-1,3-Dichloropropene	10.03	75	6075	0.628 ug/L #	58
47) Tetrachloroethene	10.86	164	21044	4.037 ug/L	89
50) Dibromochloromethane	10.86	129	19276	3.294 ug/L #	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW009286.D
Acq On : 20 Mar 2019 14:42
Operator : SY/VA
Sample : K1986-08
Misc : 5.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0Z6

Quant Time: Mar 21 10:33:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

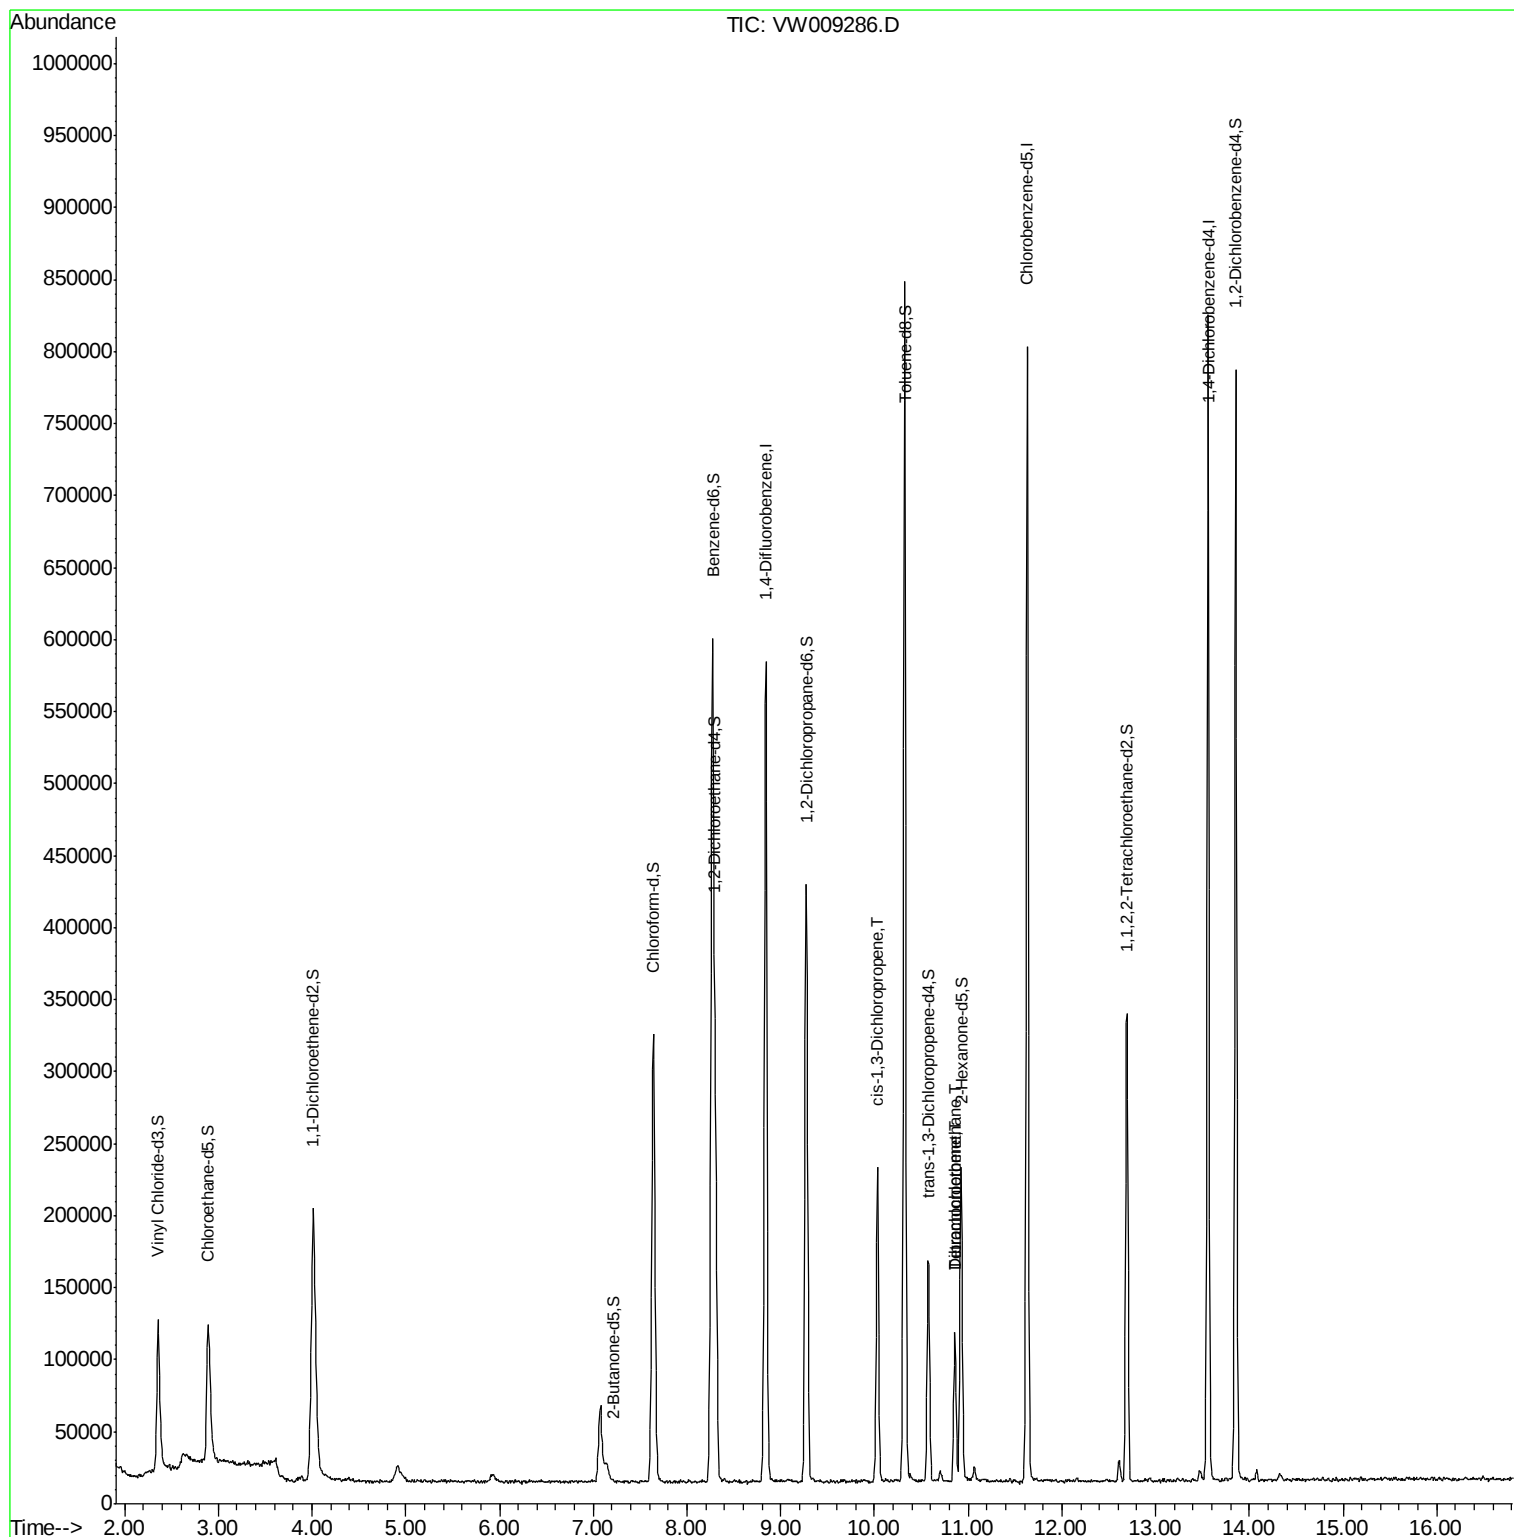

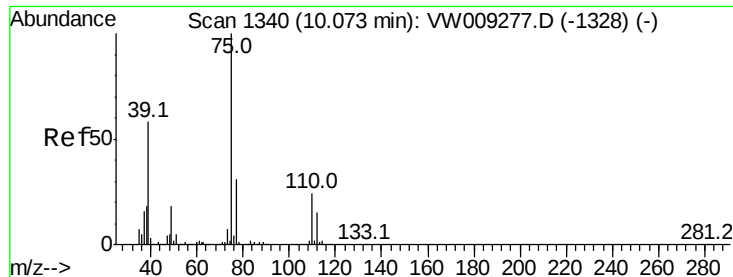

#42

cis-1,3-Dichloropropene

Concen: 0.628 ug/L

RT: 10.03 min Scan# 1333

Delta R.T. -0.04 min

Lab File: VW009286.D

Acq: 20 Mar 2019 14:42

Instrument :

MSVOA_W

ClientSampleId :





BF0Z6

Tgt Ion: 75 Resp: 6075

Ion Ratio Lower Upper

75 100

77 54.2 21.6 40.2#

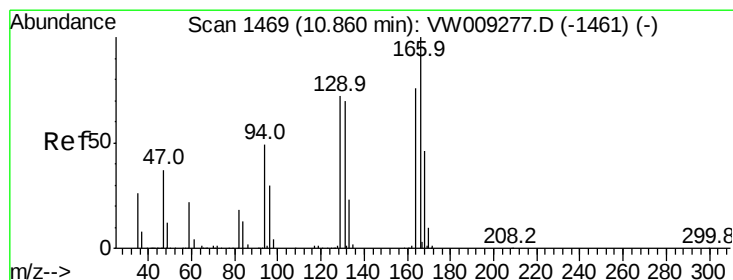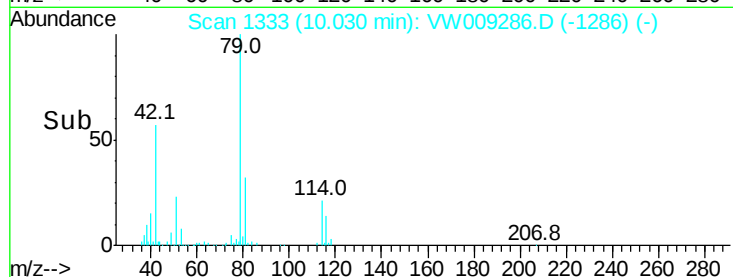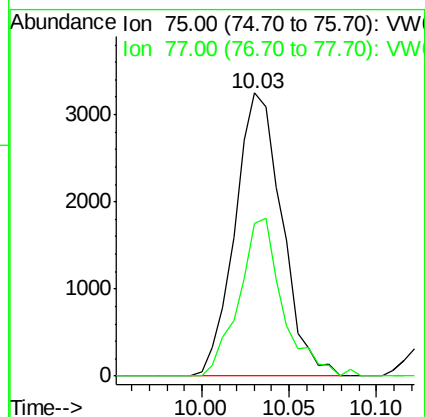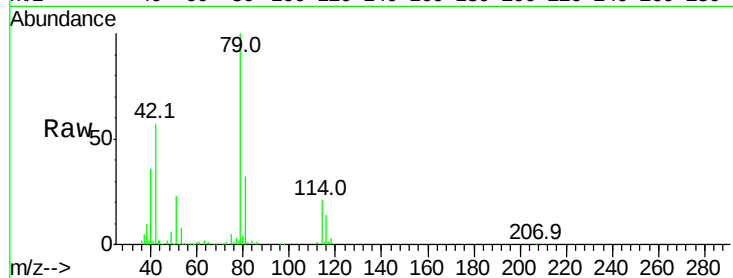

#47

Tetrachloroethene

Concen: 4.037 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VW009286.D

Acq: 20 Mar 2019 14:42

Tgt Ion: 164 Resp: 21044




Ion Ratio Lower Upper


164 100

129 90.7 66.5 123.5

131 88.0 62.6 116.3

166 106.1 91.6 170.0

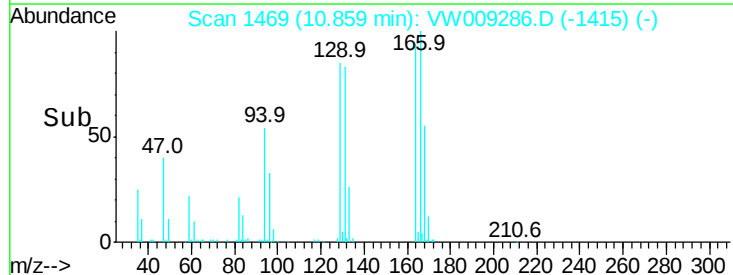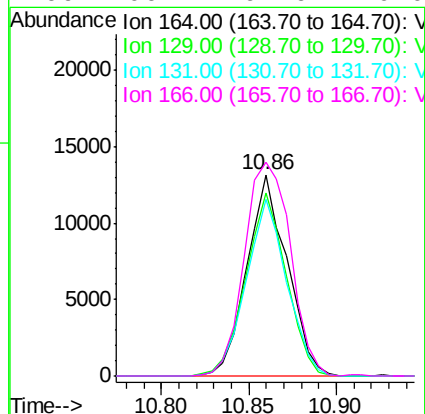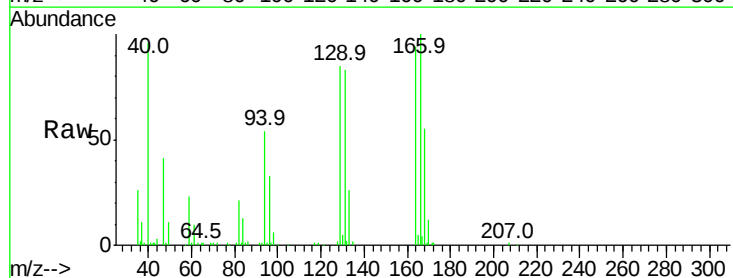

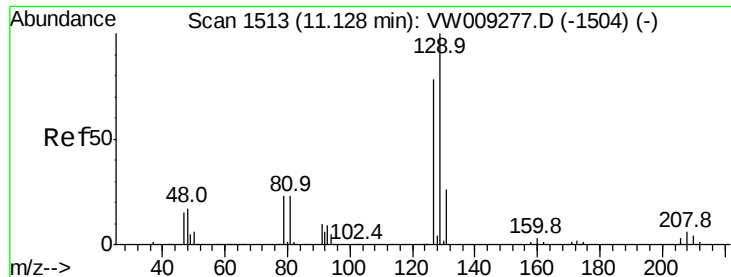

#50

Dibromochloromethane

Concen: 3.294 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. -0.27 min

Lab File: VW009286.D

Acq: 20 Mar 2019 14:42

Instrument :

MSVOA_W

ClientSampleId :


BF0Z6

Tgt Ion:129 Resp: 19276

Ion Ratio Lower Upper

129 100

127 2.0 56.8 105.6#

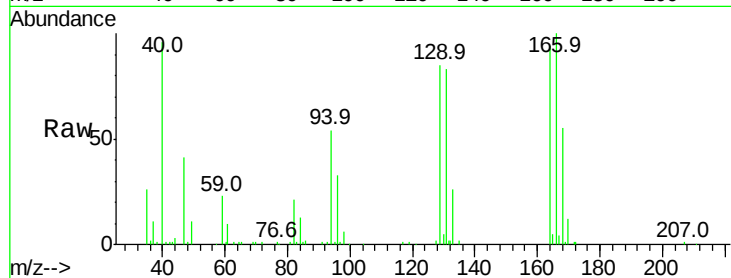

Abundance Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

