

Data File : VW009291.D
Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF121

Quant Time: Mar 21 10:34:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	361746	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	345137	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	165285	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	109245	25.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.08%
7) Chloroethane-d5	2.90	69	99259	19.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.48%
10) 1,1-Dichloroethene-d2	4.01	63	169259	18.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.48%
20) 2-Butanone-d5	7.07	46	83666	46.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.60%
24) Chloroform-d	7.65	84	231179	23.42	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.68%
26) 1,2-Dichloroethane-d4	8.47	65	147	0.02	ug/L	0.17
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.08%#
29) Benzene-d6	8.27	84	434603	22.83	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.32%
33) 1,2-Dichloropropane-d6	9.27	67	133597	23.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.48%
37) Toluene-d8	10.32	98	386188	21.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.76%
38) trans-1,3-Dichloropropene-	10.58	79	59095	20.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.32%
39) 2-Hexanone-d5	10.93	63	63077	45.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	130842	23.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	151792	23.95	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.80%


Target Compounds					Qvalue
13) Acetone	4.12	43	2119	1.445 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW009291.D
Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF121

Quant Time: Mar 21 10:34:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

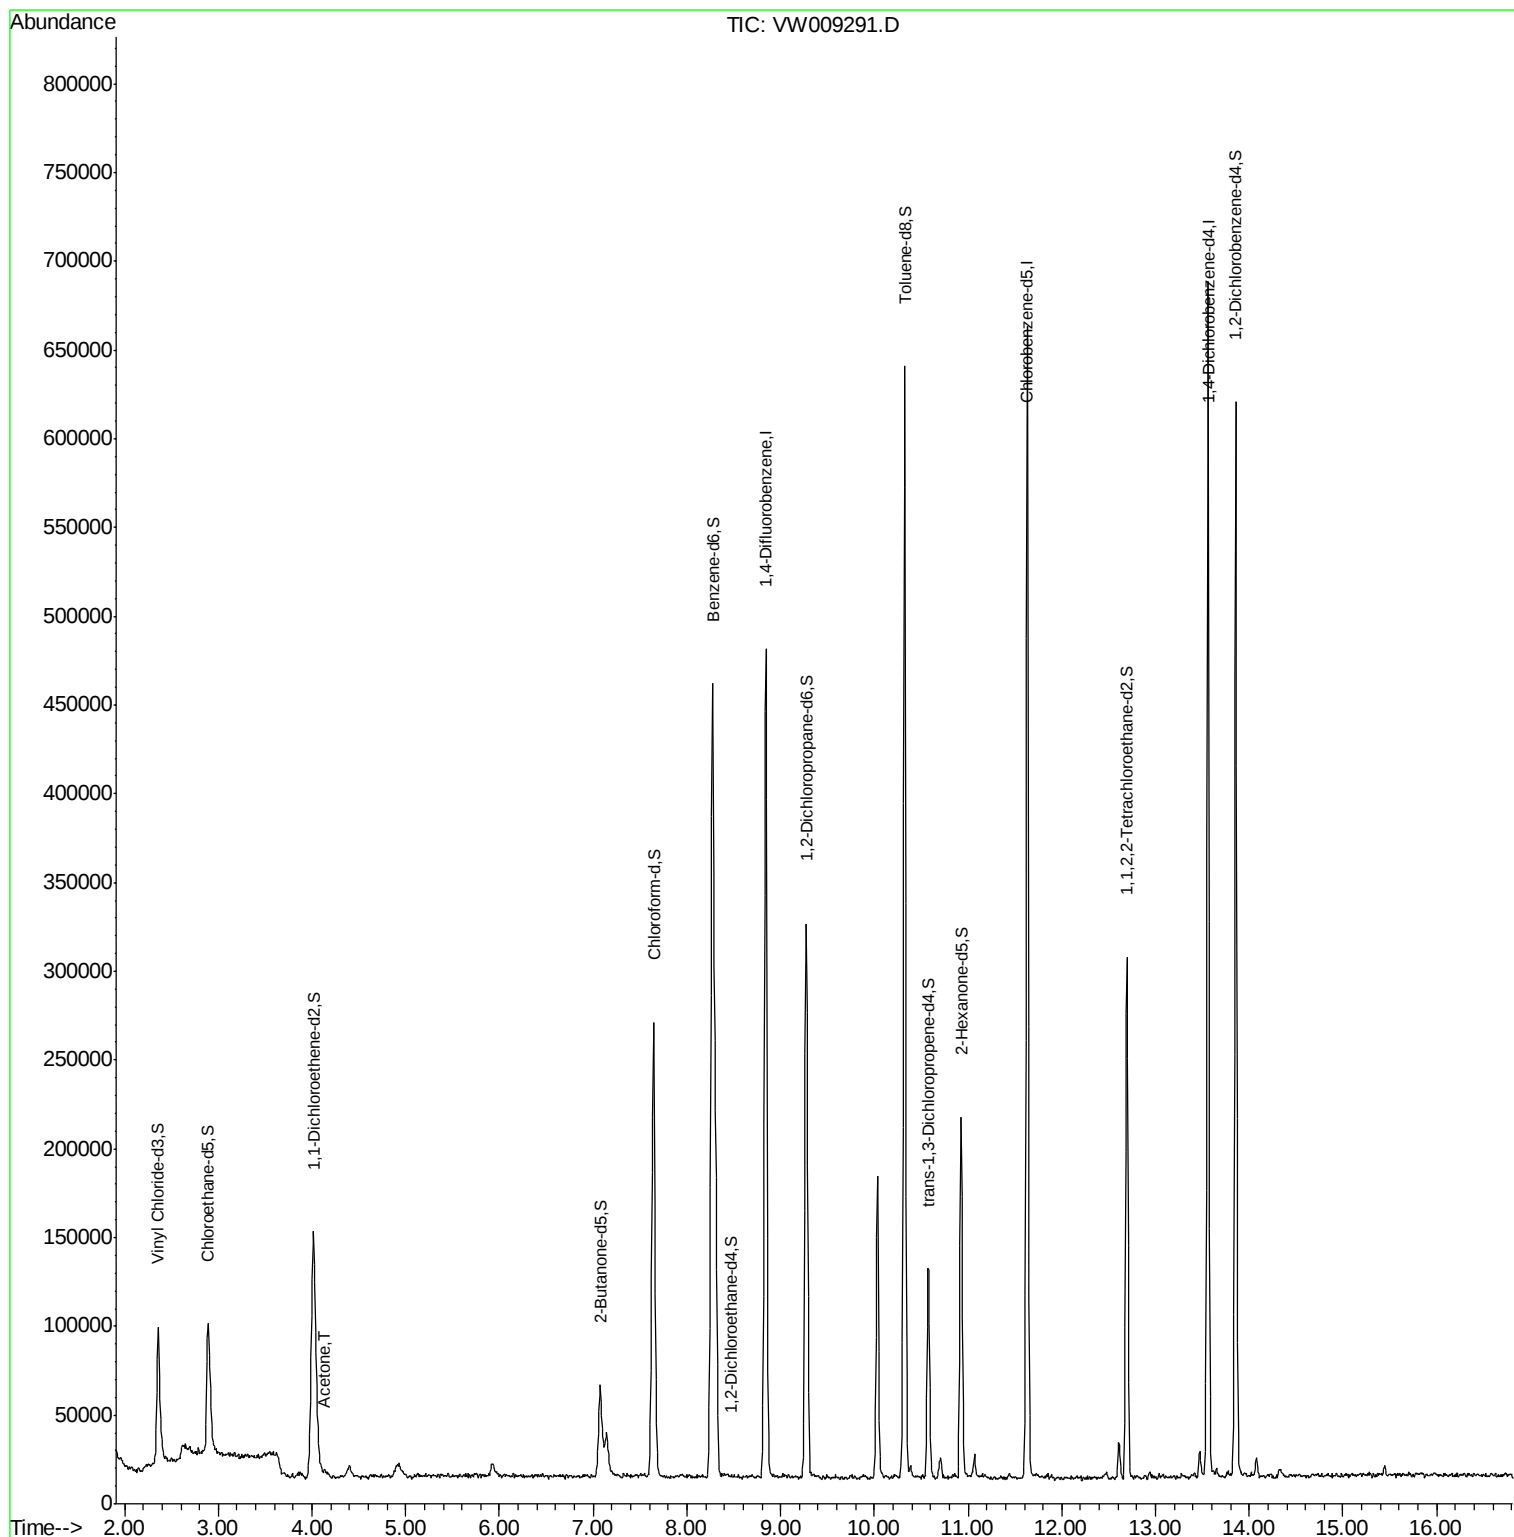

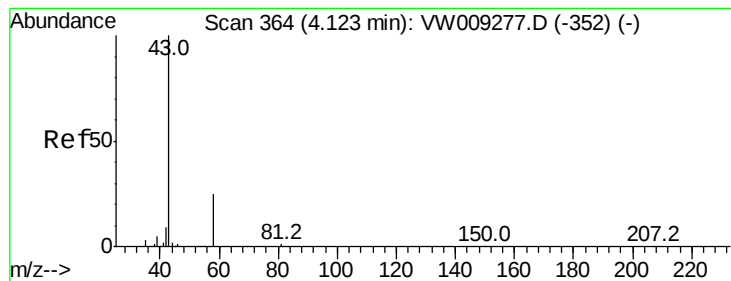

#13
 Acetone
 Concen: 1.445 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.00 min
 Lab File: VW009291.D
 Acq: 20 Mar 2019 16:57

Instrument :
 MSVOA_W
 ClientSampleId :
 BF121

Tgt Ion: 43 Resp: 2119
 Ion Ratio Lower Upper
 43 100
 58 21.1 0.0 56.2

