

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009291.D
Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF121

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:27 AM

Quant Time: Mar 21 11:29:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

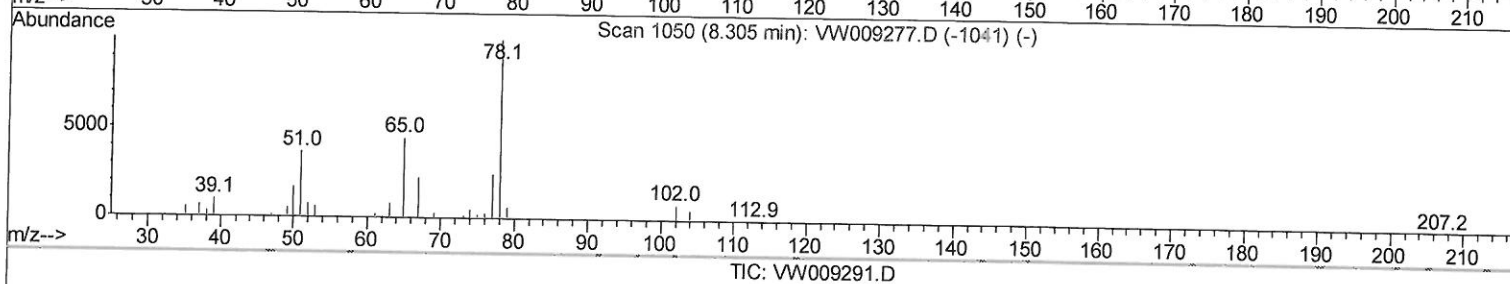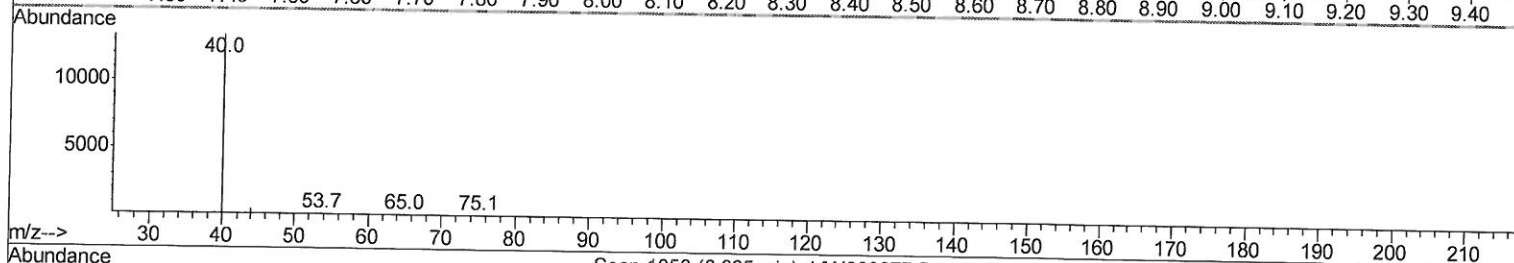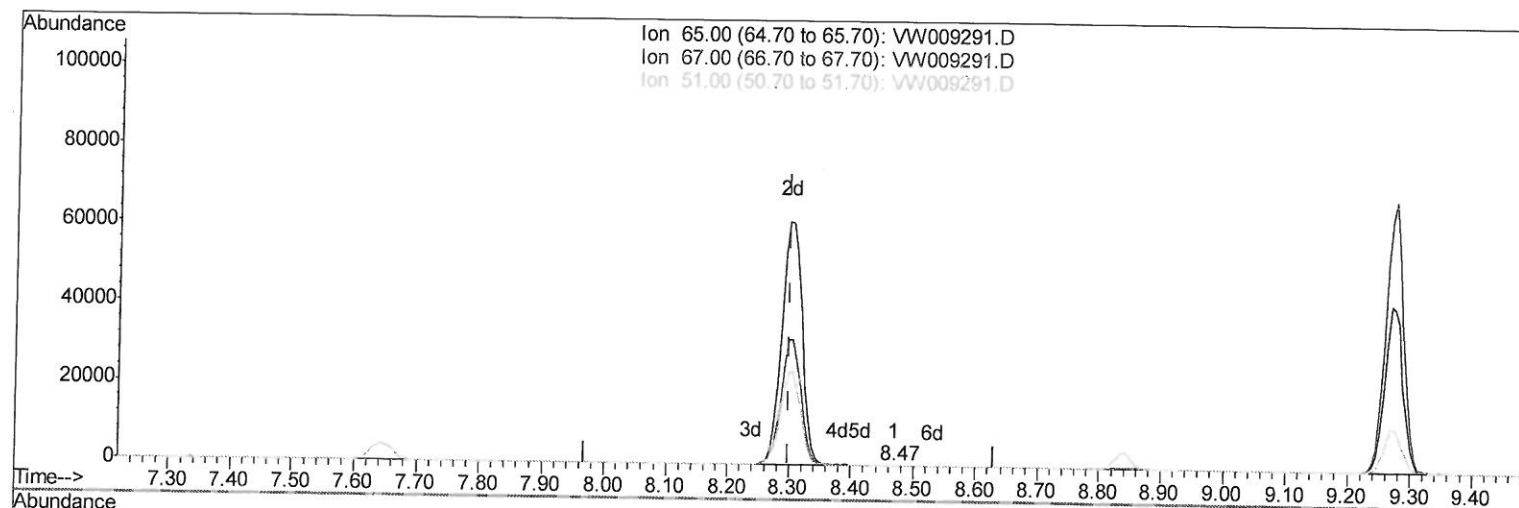

(26) 1,2-Dichloroethane-d4 (S)

8.470min (+0.171) 0.02ug/L

response 147

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	53.74
51.00	97.70	82.31
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009291.D
Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF121

Quant Time: Mar 21 11:29:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:27 AM

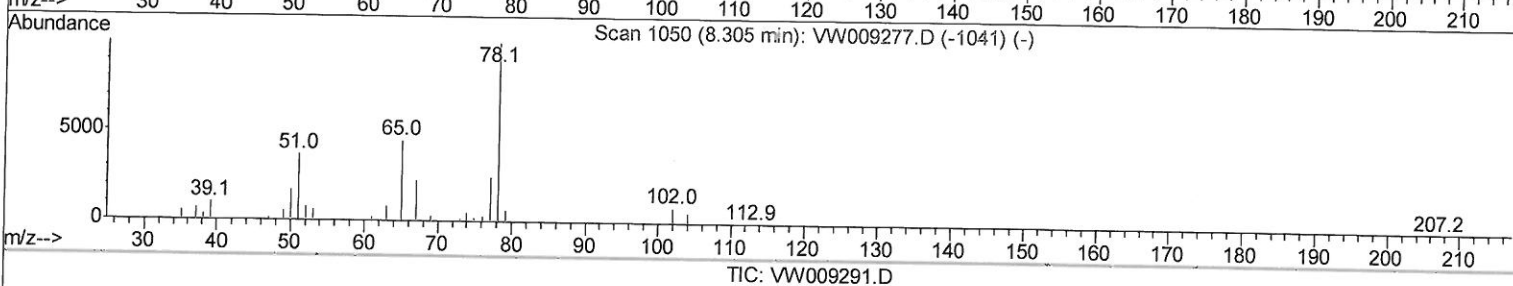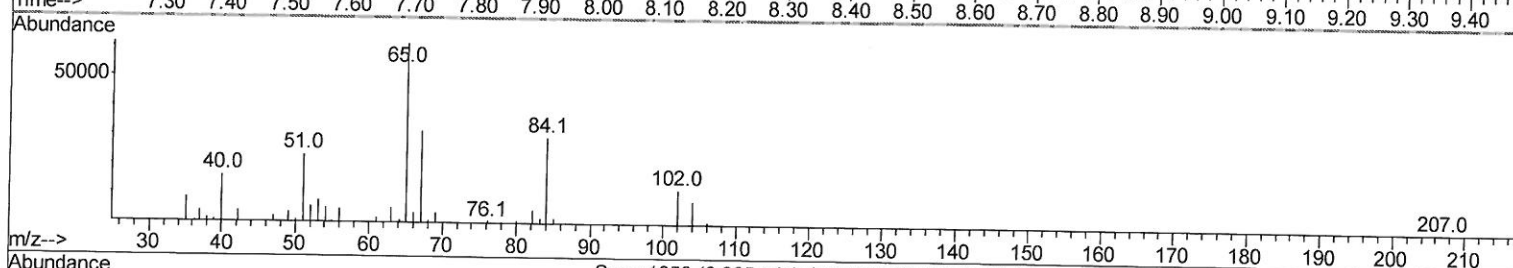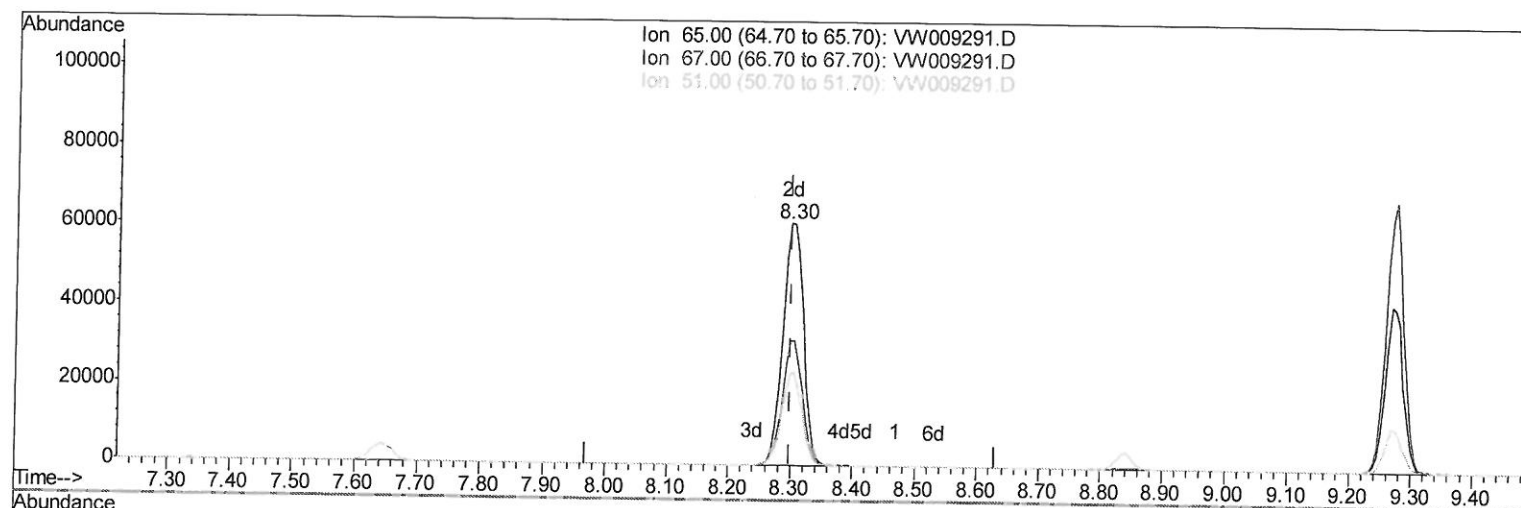

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+0.000) 23.31ug/L m

503/24/19 54

response 138631

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	0.06#
51.00	97.70	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (QT Reviewed)

Data File : VW009291.D
Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF121

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:27 AM

Quant Time: Mar 21 14:10:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	361746	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	345137	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	165285	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	109245	25.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.08%
7) Chloroethane-d5	2.90	69	99259	19.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.48%
10) 1,1-Dichloroethene-d2	4.01	63	169259	18.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.48%
20) 2-Butanone-d5	7.07	46	83666	46.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.60%
24) Chloroform-d	7.65	84	231179	23.42	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.68%
26) 1,2-Dichloroethane-d4	8.30	65	138631m	23.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.24%
29) Benzene-d6	8.27	84	434603	22.83	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.32%
33) 1,2-Dichloropropane-d6	9.27	67	133597	23.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.48%
37) Toluene-d8	10.32	98	386188	21.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.76%
38) trans-1,3-Dichloropropene-	10.58	79	59095	20.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.32%
39) 2-Hexanone-d5	10.93	63	63077	45.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	130842	23.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.96%
61) 1,2-Dichlorobenzene-d4	13.86	152	151792	23.95	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.80%

83/25/1957

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Data File : VW009291.D Quantitation Report (QT Reviewed)


Acq On : 20 Mar 2019 16:57
Operator : SY/VA
Sample : K1986-13
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF121

Quant Time: Mar 21 14:10:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:27 AM

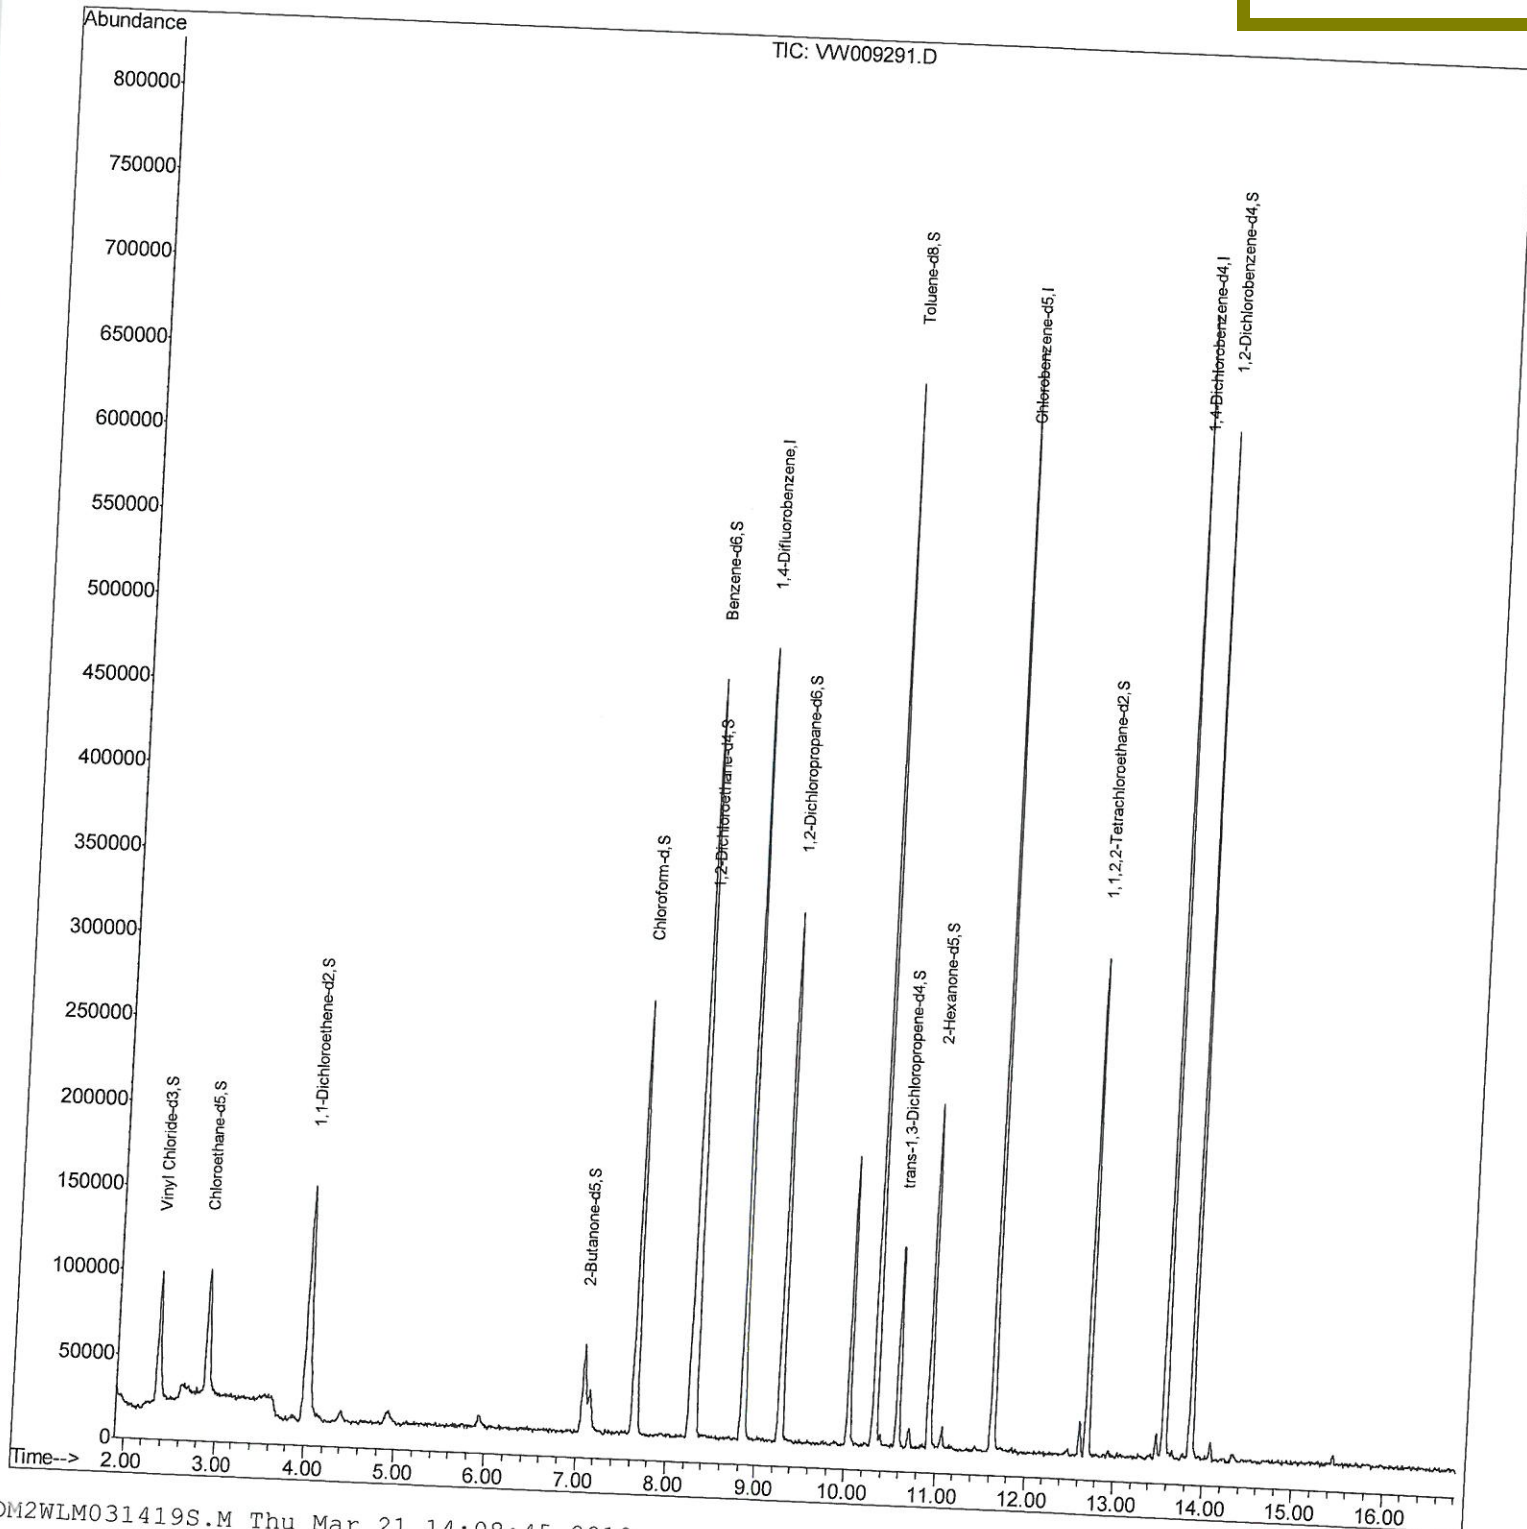

SOM2WLM031419S.M Thu Mar 21 14:08:45 2019