

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009294.D
Acq On : 20 Mar 2019 18:18
Operator : SY/VA
Sample : K1986-16
Misc : 5.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF124

Quant Time: Mar 21 11:34:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:28 AM

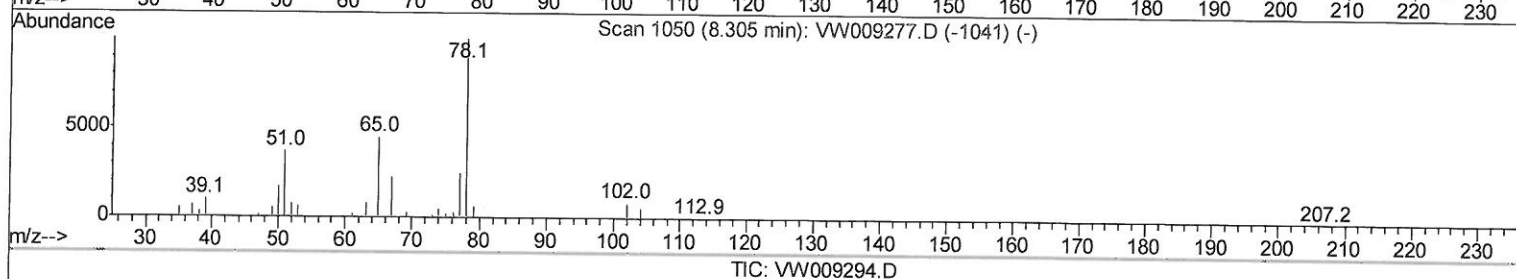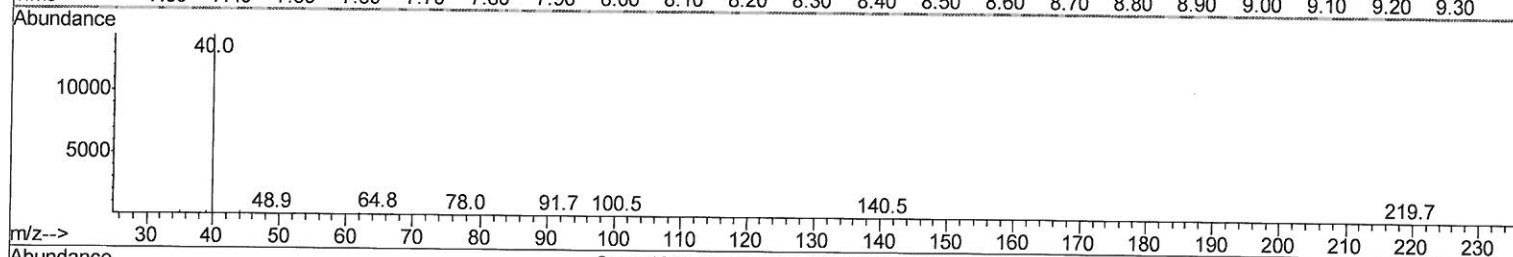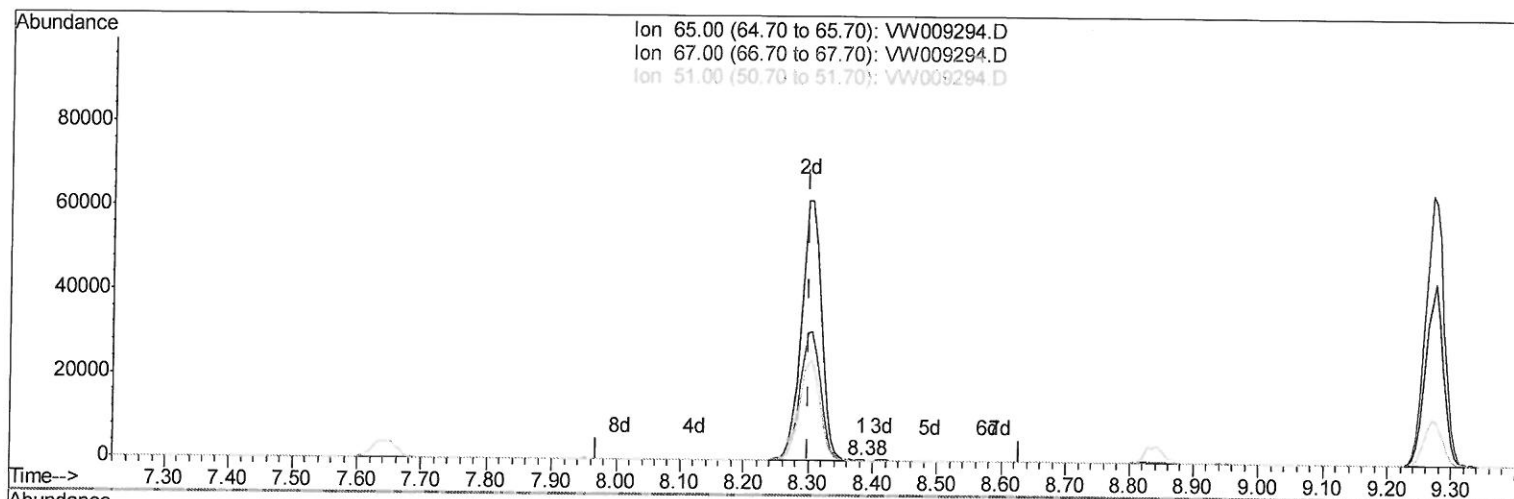

(26) 1,2-Dichloroethane-d4 (S)

8.384min (+0.085) 0.03ug/L

response 177

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	56.50
51.00	97.70	75.14
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009294.D
Acq On : 20 Mar 2019 18:18
Operator : SY/VA
Sample : K1986-16
Misc : 5.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF124

Quant Time: Mar 21 11:34:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:28 AM

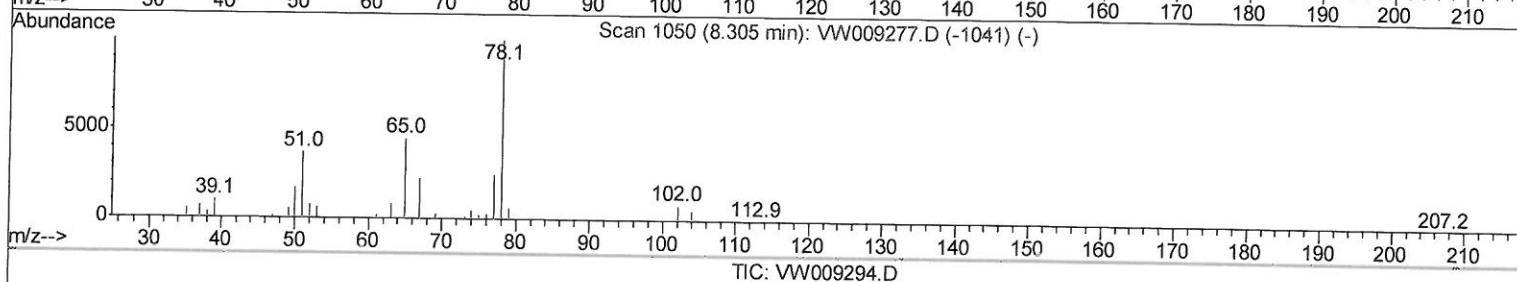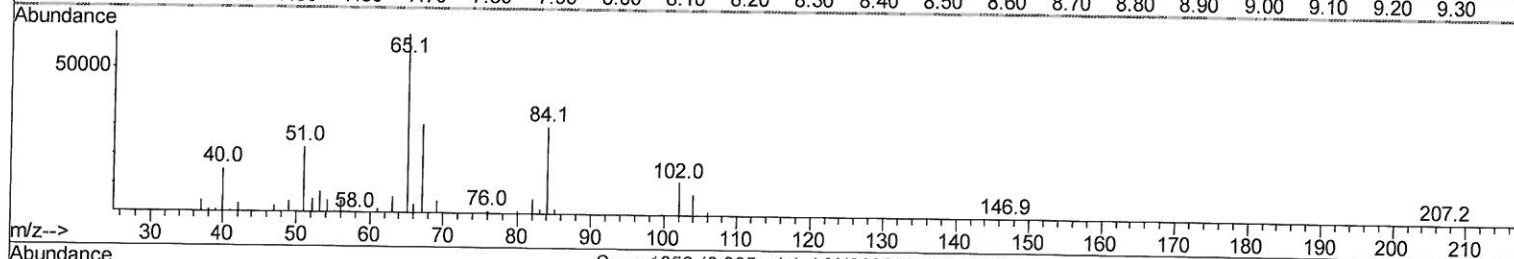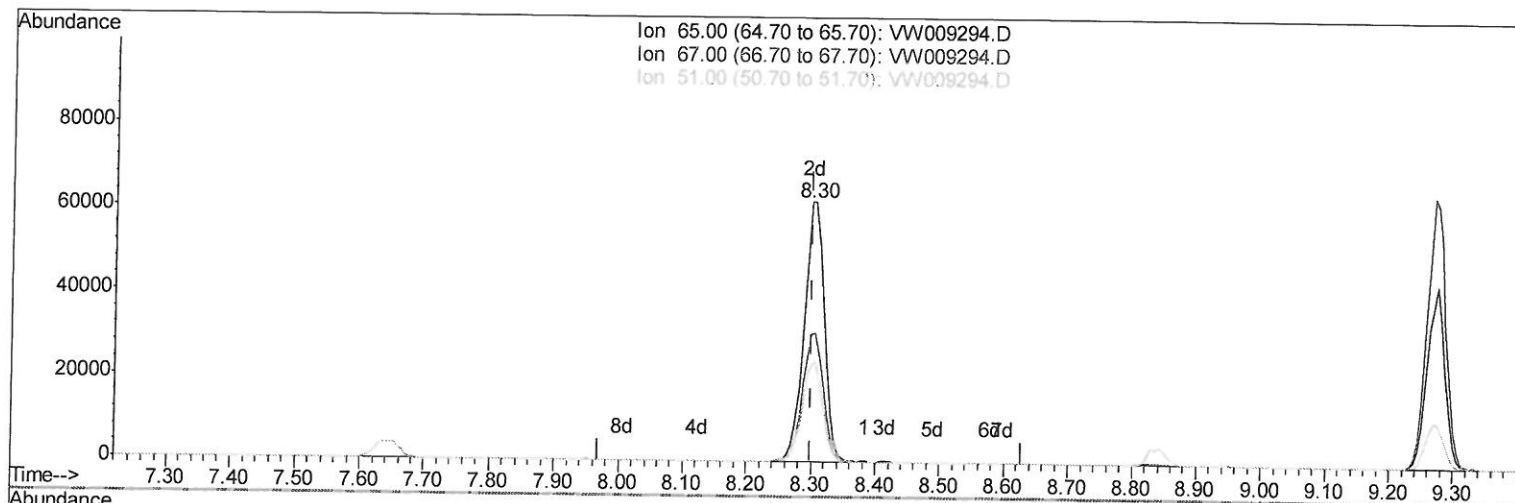

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.000) 22.55ug/L m

203/24/19 Sy

response 134562

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	0.07#
51.00	97.70	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (QT Reviewed)

Data File : VW009294.D
Acq On : 20 Mar 2019 18:18
Operator : SY/VA
Sample : K1986-16
Misc : 5.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF124

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:28 AM

Quant Time: Mar 21 14:11:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	362944	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	349322	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	163963	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	107035	24.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.72%
7) Chloroethane-d5	2.89	69	101808	20.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.24%
10) 1,1-Dichloroethene-d2	4.01	63	166489	17.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.04%
20) 2-Butanone-d5	7.08	46	70894	39.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.04%
24) Chloroform-d	7.64	84	226833	22.90	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	8.30	65	134562m	22.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.20%
29) Benzene-d6	8.27	84	426011	22.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.44%
33) 1,2-Dichloropropane-d6	9.27	67	129087	22.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.24%
37) Toluene-d8	10.32	98	382808	21.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.96%
38) trans-1,3-Dichloropropene-	10.57	79	55987	19.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.08%
39) 2-Hexanone-d5	10.93	63	53688	38.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	118759	20.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	147128	23.40	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.60%

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (QT Reviewed)
Data File : VW009294.D
Acq On : 20 Mar 2019 18:18
Operator : SY/VA
Sample : K1986-16
Misc : 5.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF124

Quant Time: Mar 21 14:11:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 10:17:44 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:28 AM

