


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032019\
Data File : VW009315.D
Acq On : 21 Mar 2019 05:00
Operator : SY/VA
Sample : K1988-16
Misc : 6.23G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 07:35:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 12:20:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
BF0C8

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:38 AM

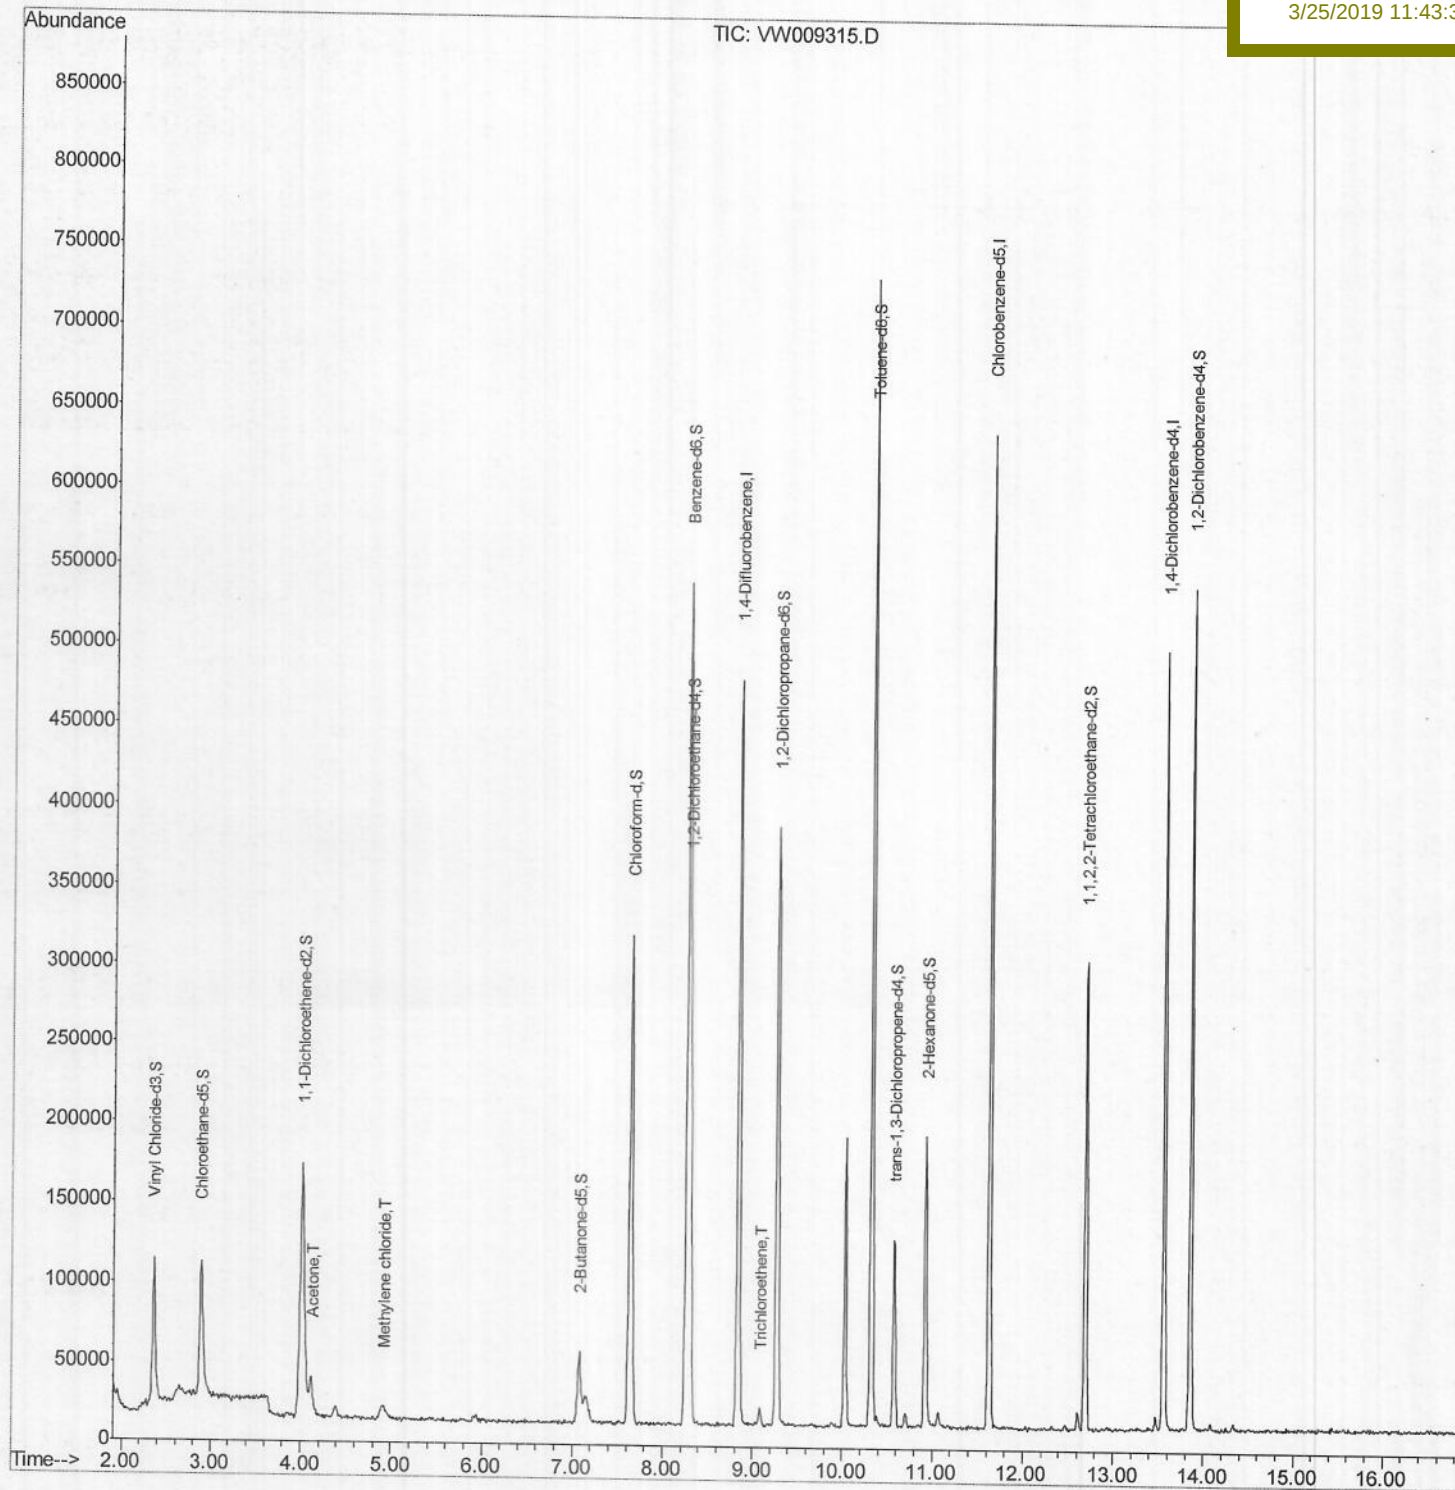

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009315.D
Acq On : 21 Mar 2019 05:00
Operator : SY/VA
Sample : K1988-16
Misc : 6.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 12:25:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 12:20:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
BF0C8

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:38 AM

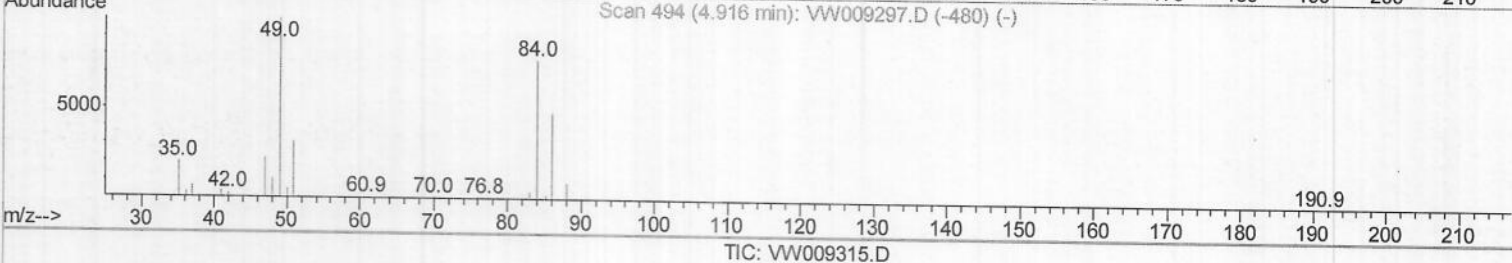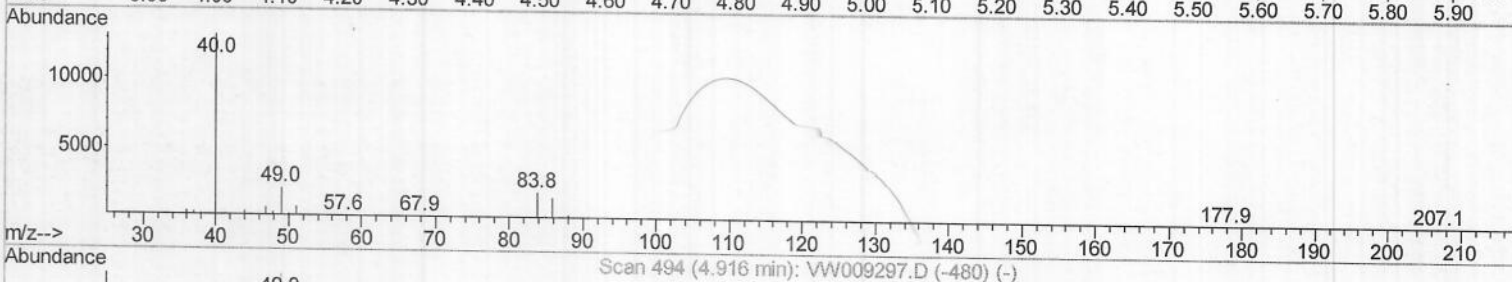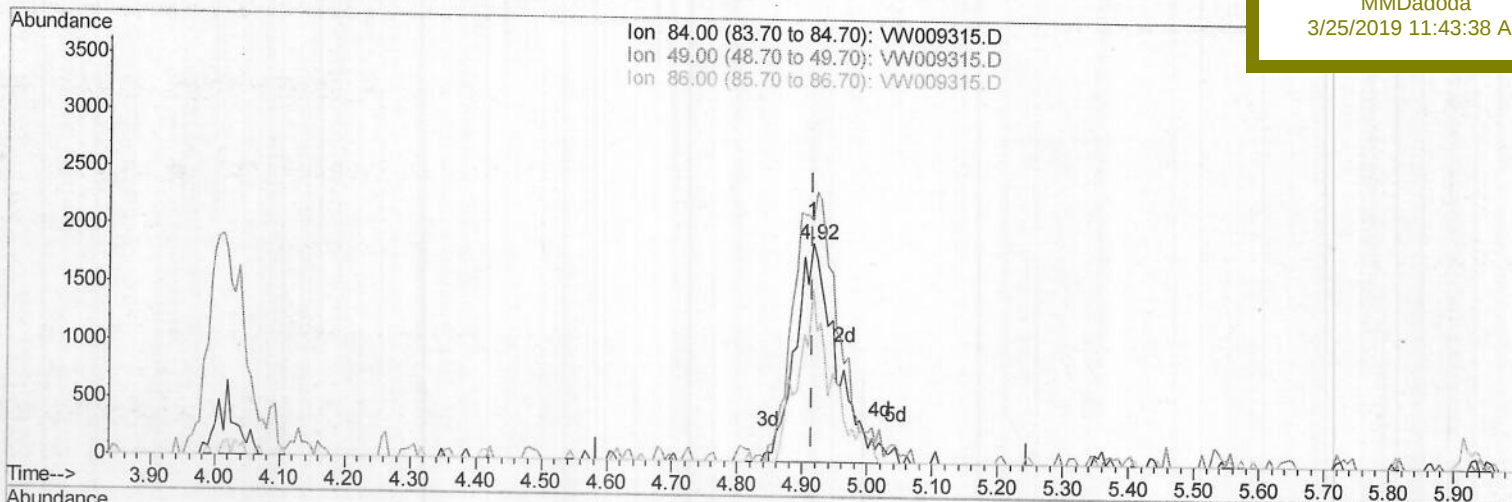

(16) Methylene chloride (T)

4.915min (-0.000) 1.54ug/L m

response 8275

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	110.63
86.00	63.50	80.11
0.00	0.00	0.00

03/27/19
SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032019\
Quantitation Report (Qedit)




Data File : VW009315.D
Acq On : 21 Mar 2019 05:00
Operator : SY/VA
Sample : K1988-16
Misc : 6.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 12:25:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 12:20:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
BF0C8

Manual Integrations
APPROVED

MMDadoda
3/25/2019 11:43:38 AM

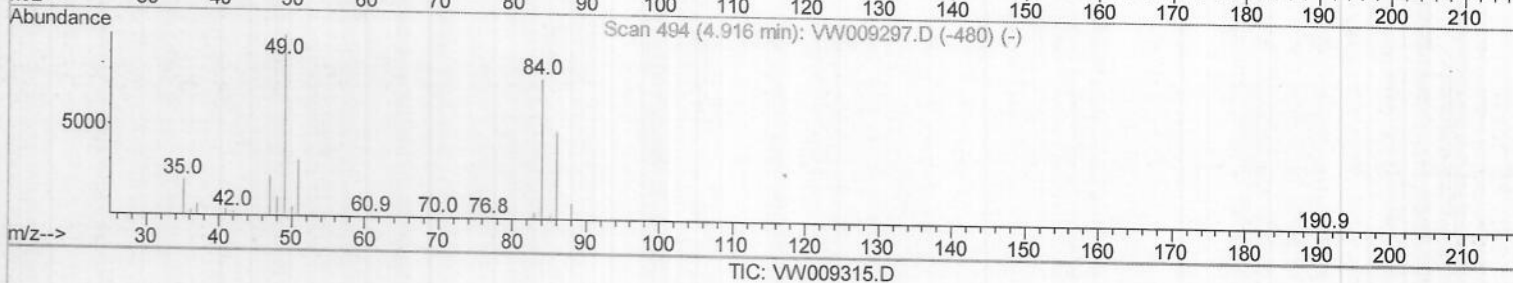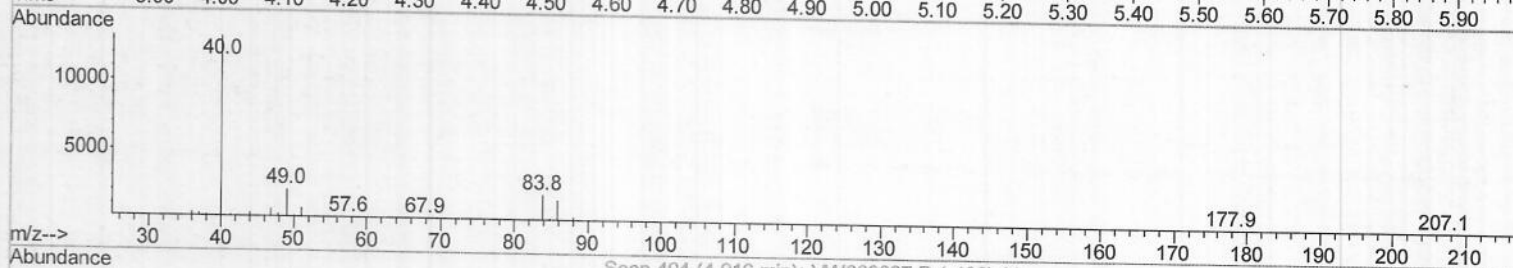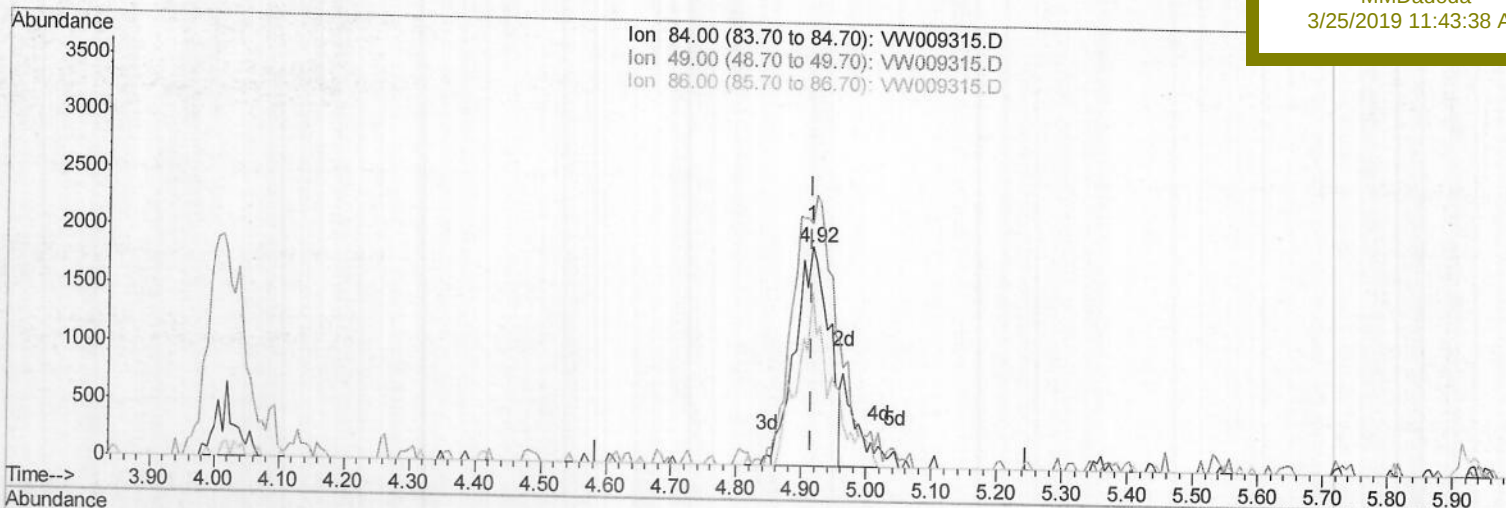

(16) Methylene chloride (T)

4.915min (-0.000) 1.27ug/L

response 6828

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	110.63
86.00	63.50	80.11
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032019\
 Data File : VW009315.D
 Acq On : 21 Mar 2019 05:00
 Operator : SY/VA
 Sample : K1988-16
 Misc : 6.23G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0C8

Quant Time: Apr 05 07:35:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 12:20:05 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 11:43:38 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	367824	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	331987	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	118507	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	125329	28.51	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	114.04%	
7) Chloroethane-d5	2.89	69	121089	23.54	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	94.16%	
10) 1,1-Dichloroethene-d2	4.02	63	189252	19.92	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	79.68%	
20) 2-Butanone-d5	7.08	46	73892	40.65	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	81.30%	
24) Chloroform-d	7.65	84	276120	27.51	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	110.04%	
26) 1,2-Dichloroethane-d4	8.30	65	157404	26.03	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	104.12%	
29) Benzene-d6	8.27	84	513269	28.03	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	112.12%	
33) 1,2-Dichloropropane-d6	9.27	67	162401	29.53	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	118.12%	
37) Toluene-d8	10.32	98	446081	26.35	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	105.40%	
38) trans-1,3-Dichloropropene-	10.58	79	58673	21.24	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	84.96%	
39) 2-Hexanone-d5	10.93	63	53391	40.09	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	80.18%	
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129138	23.84	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	95.36%	
61) 1,2-Dichlorobenzene-d4	13.86	152	134306	29.56	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	118.24%	

Target Compounds

13) Acetone	4.12	43	38731	25.982	ug/L	Ovalue
16) Methylene chloride	4.92	84	8275m	1.543	ug/L	99
35) Trichloroethene	9.09	95	3051	0.630	ug/L	# 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed