

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
 Data File : VW009348.D
 Acq On : 22 Mar 2019 15:04
 Operator : SY/VA
 Sample : K2017-18
 Misc : 5.33G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0E4

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 8:29:33 AM

Quant Time: Mar 23 00:18:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 23 00:14:14 2019
 Response via : Initial Calibration

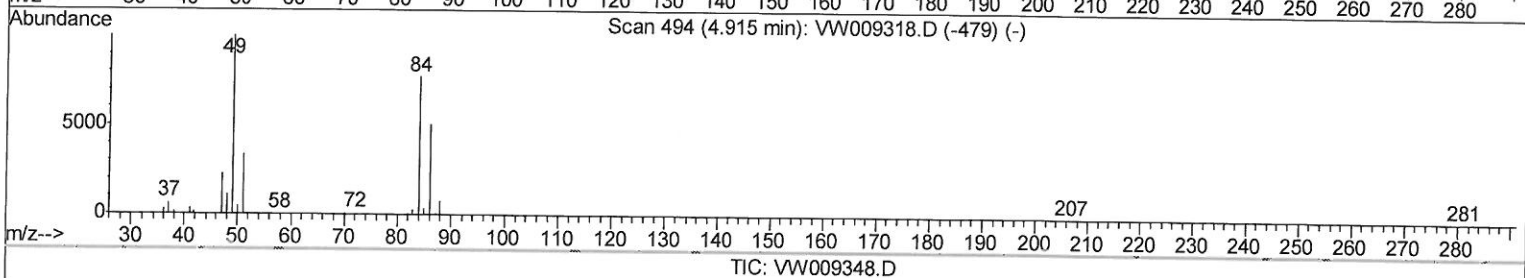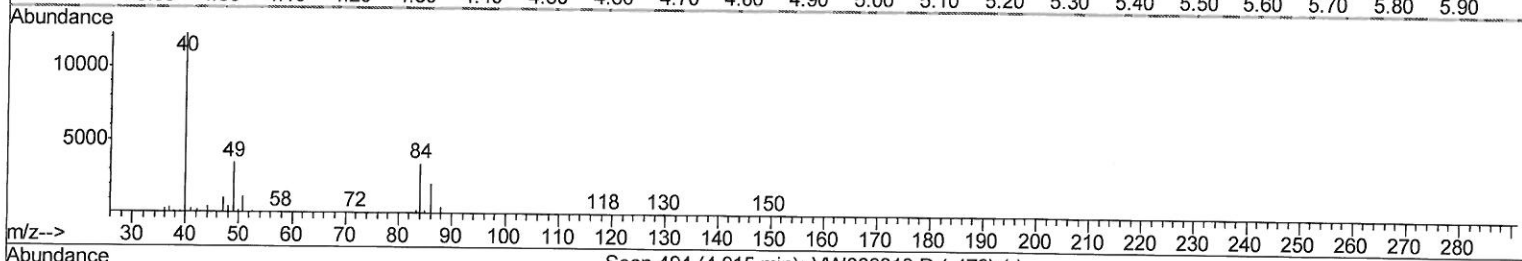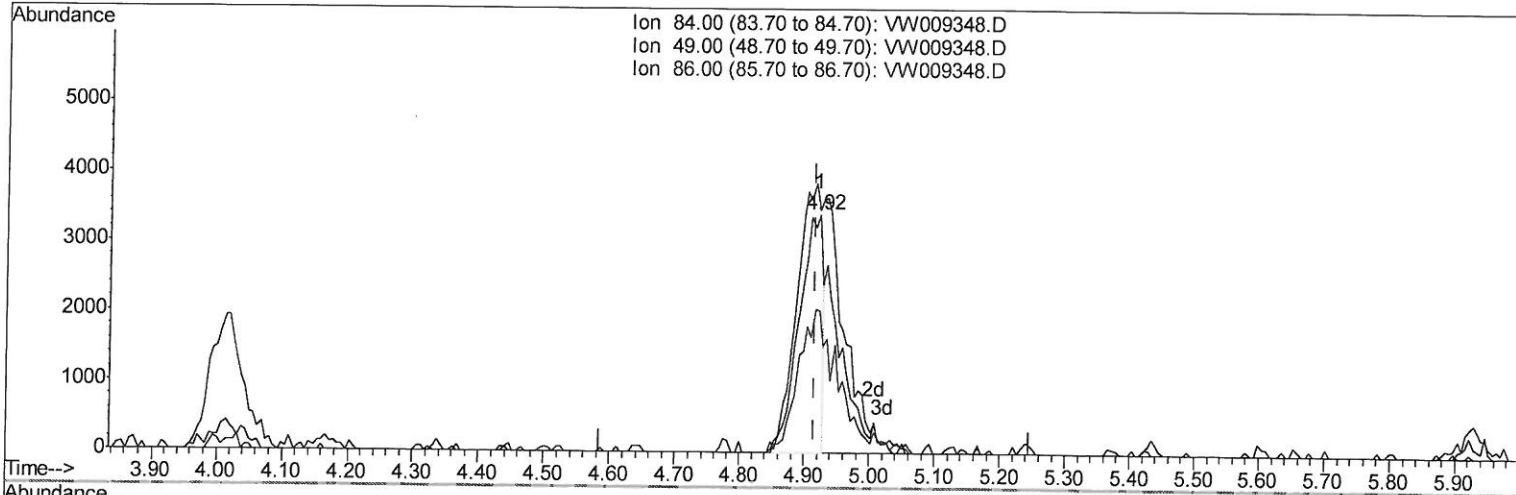

TIC: VW009348.D

(16) Methylene chloride (T)

4.922min (+0.006) 1.44ug/L

response 8663

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	102.12
86.00	63.50	59.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
 Data File : VW009348.D
 Acq On : 22 Mar 2019 15:04
 Operator : SY/VA
 Sample : K2017-18
 Misc : 5.33G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0E4

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 8:29:33 AM

Quant Time: Mar 23 00:18:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 23 00:14:14 2019
 Response via : Initial Calibration

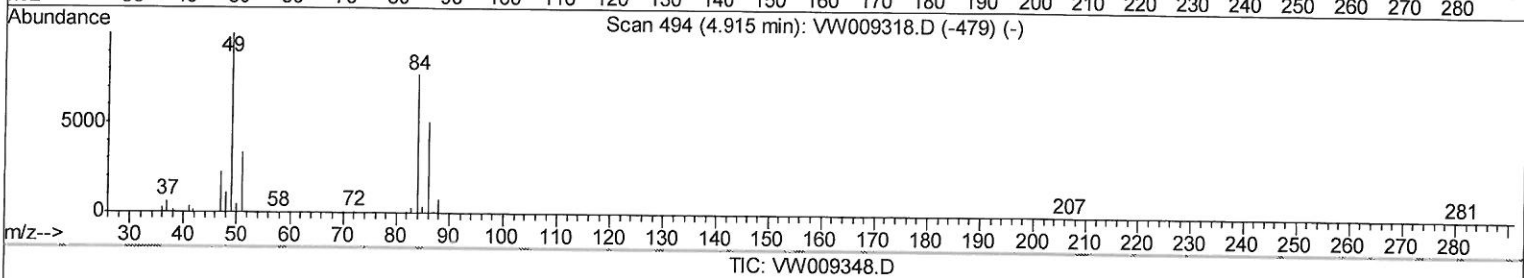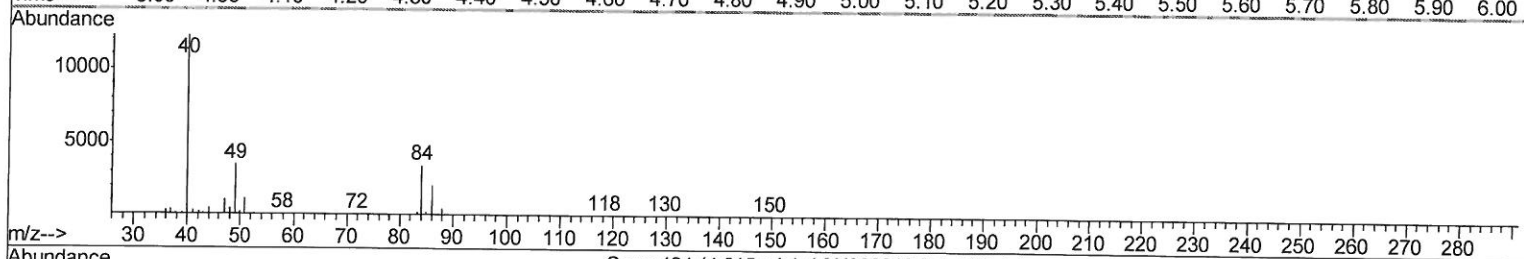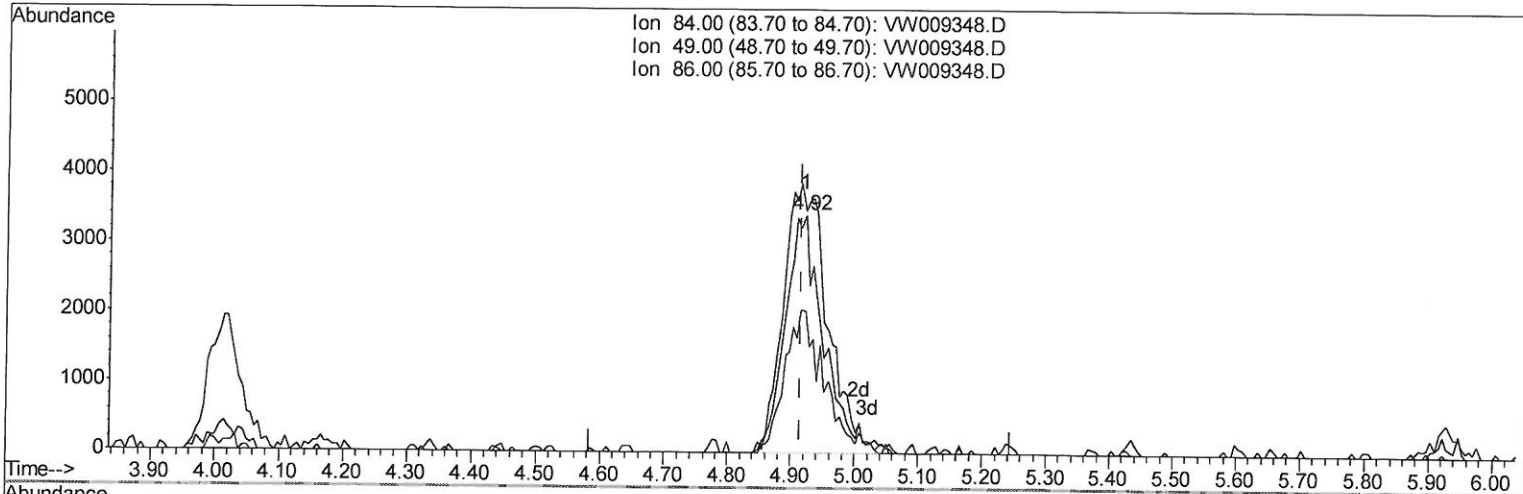

(16) Methylene chloride (T)

4.922min (+0.006) 2.34ug/L m

507/24/19 SY

response 14102

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	102.12
86.00	63.50	59.55
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
 Data File : VW009348.D
 Acq On : 22 Mar 2019 15:04
 Operator : SY/VA
 Sample : K2017-18
 Misc : 5.33G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0E4

Quant Time: Mar 23 00:52:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 23 00:14:14 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 3/25/2019 8:29:33 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	413687	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	397903	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	184950	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	105534	21.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.40%
7) Chloroethane-d5	2.89	69	108982	18.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.36%
10) 1,1-Dichloroethene-d2	4.01	63	167597	15.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.76%
20) 2-Butanone-d5	7.08	46	109660	53.64	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.28%
24) Chloroform-d	7.64	84	258402	22.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.56%
26) 1,2-Dichloroethane-d4	8.31	65	164972	24.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.04%
29) Benzene-d6	8.27	84	467207	21.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.16%
33) 1,2-Dichloropropane-d6	9.27	67	151449	22.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.92%
37) Toluene-d8	10.32	98	416301	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.08%
38) trans-1,3-Dichloropropene-	10.58	79	68714	20.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.04%
39) 2-Hexanone-d5	10.93	63	80074	50.16	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.32%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	162379	25.02	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.08%
61) 1,2-Dichlorobenzene-d4	13.85	152	172260	24.29	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.16%

Target Compounds

16) Methylene chloride	4.92	84	14102m)	2.338	ug/L	Qvalue
22) cis-1,2-Dichloroethene	7.17	96	5801	1.000	ug/L	88
35) Trichloroethene	9.09	95	6096	1.050	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Data File : VW009348.D
Acq On : 22 Mar 2019 15:04
Operator : SY/VA
Sample : K2017-18
Misc : 5.33G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF0E4

Quant Time: Mar 23 00:52:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 00:14:14 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:33 AM

