

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009371.D
Acq On : 23 Mar 2019 03:55
Operator : SY/VA
Sample : K2031-15
Misc : 4.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5S5

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:46 AM

Quant Time: Mar 23 06:20:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

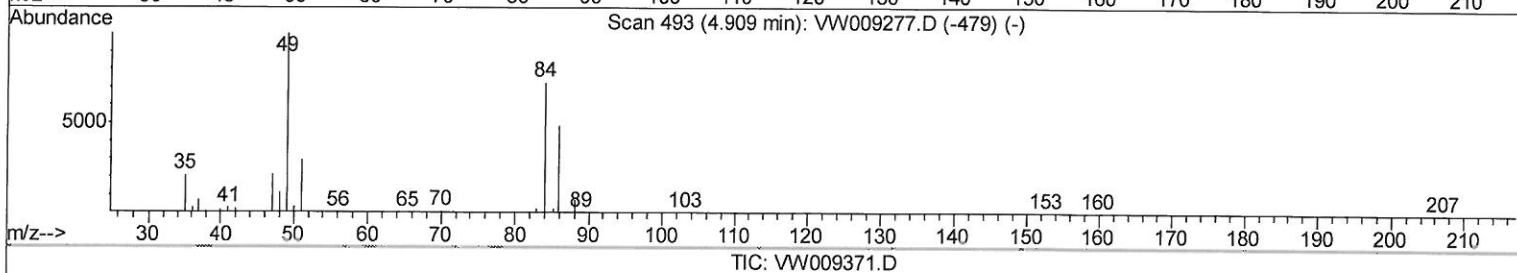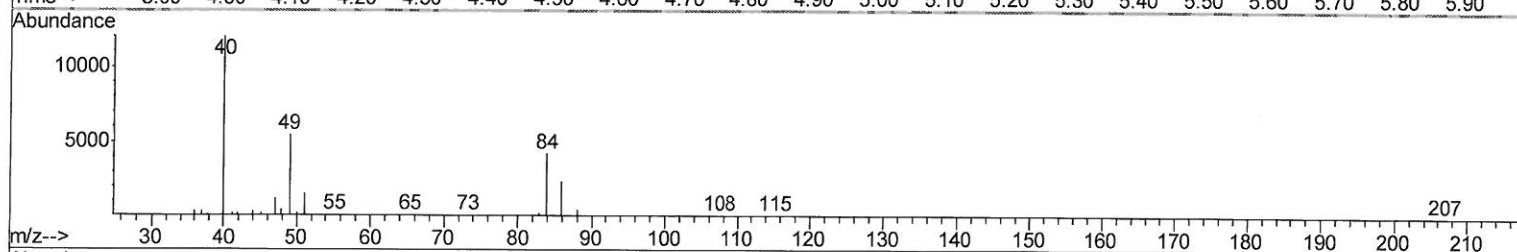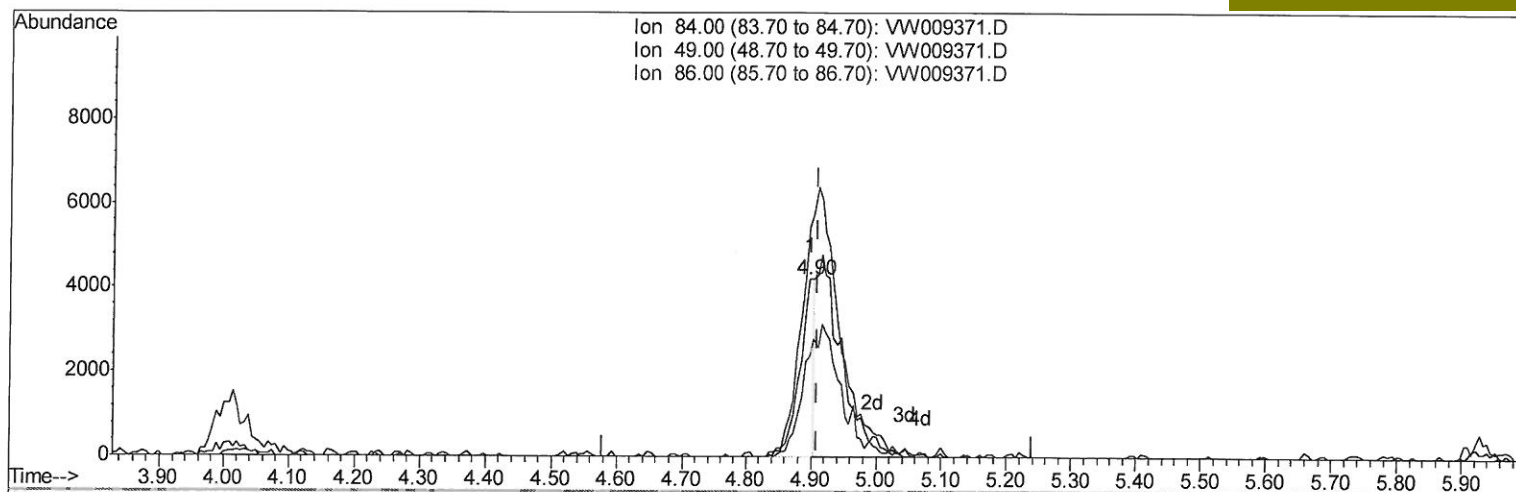

(16) Methylene chloride (T)

4.897min (-0.012) 1.50ug/L

response 6680

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	128.94
86.00	63.50	55.64
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009371.D
Acq On : 23 Mar 2019 03:55
Operator : SY/VA
Sample : K2031-15
Misc : 4.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5S5

Quant Time: Mar 23 06:20:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:46 AM

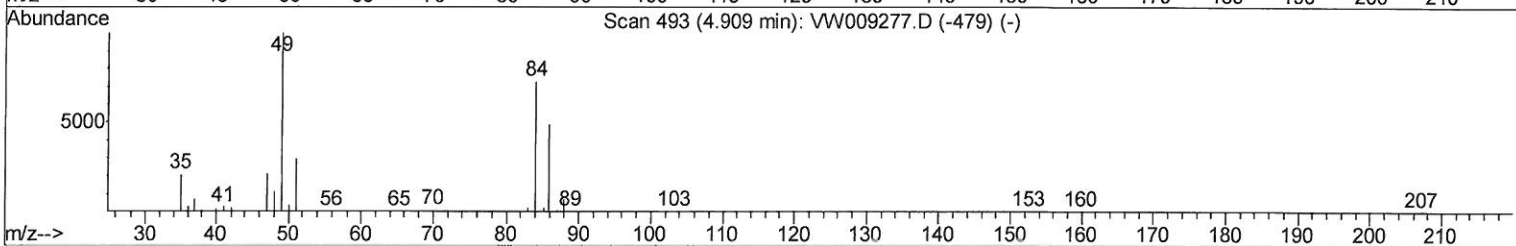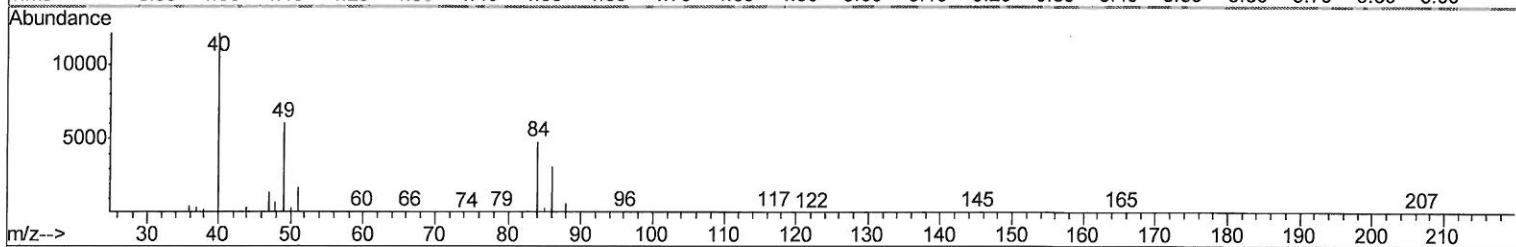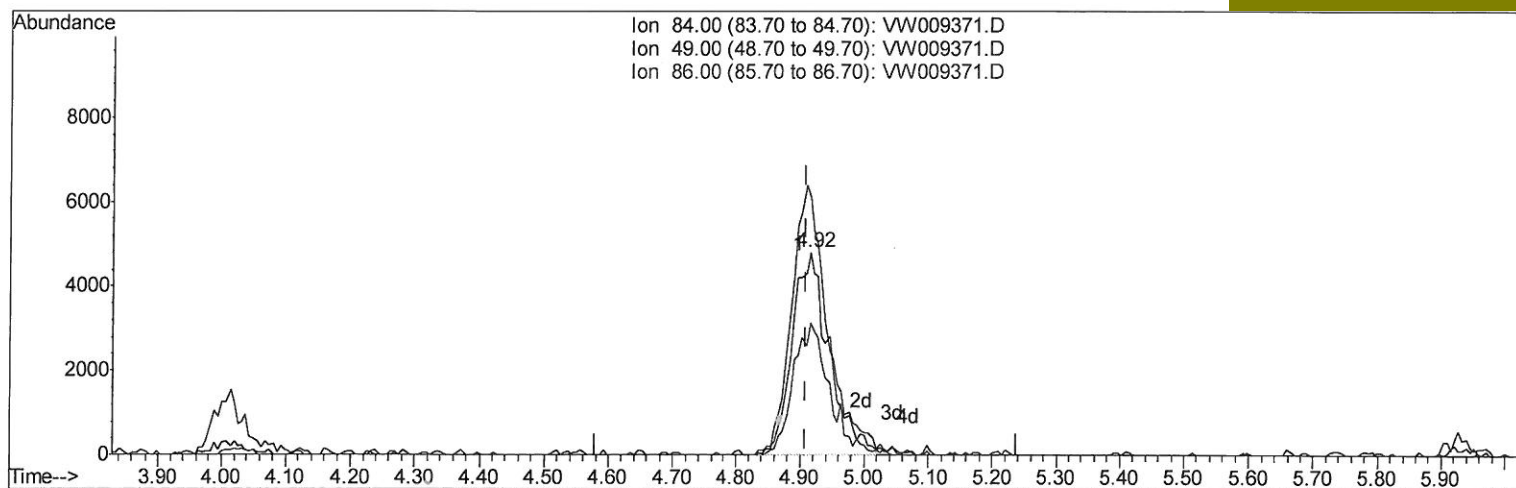

TIC: VW009371.D

(16) Methylene chloride (T)

4.916min (+0.006) 4.33ug/L m

207/24/19 SY

response 19328

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	127.20
86.00	63.50	65.57
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)

Data File : VW009371.D
Acq On : 23 Mar 2019 03:55
Operator : SY/VA
Sample : K2031-15
Misc : 4.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sample Id :
BF5S5

Quant Time: Mar 23 06:36:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:46 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	306108	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	293750	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	123024	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	76394	20.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.52%
7) Chloroethane-d5	2.89	69	79852	18.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.64%
10) 1,1-Dichloroethene-d2	4.01	63	122161	15.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.80%
20) 2-Butanone-d5	7.08	46	85533	56.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.08%
24) Chloroform-d	7.65	84	203774	24.39	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.56%
26) 1,2-Dichloroethane-d4	8.30	65	130937	26.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.08%
29) Benzene-d6	8.27	84	355431	21.94	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.76%
33) 1,2-Dichloropropane-d6	9.27	67	119953	24.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.60%
37) Toluene-d8	10.32	98	301417	20.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.48%
38) trans-1,3-Dichloropropene-	10.57	79	50861	20.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.24%
39) 2-Hexanone-d5	10.93	63	63224	53.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	127114	26.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.12%
61) 1,2-Dichlorobenzene-d4	13.86	152	114958	24.37	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.48%

Target Compounds

13) Acetone	4.12	43	28388	22.883	ug/L	83
16) Methylene chloride	4.92	84	19328m	> 4.330	ug/L	

Qvalue
03/24/19 54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)

Data File : VW009371.D
Acq On : 23 Mar 2019 03:55
Operator : SY/VA
Sample : K2031-15
Misc : 4.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5S5

Quant Time: Mar 23 06:36:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:46 AM

