

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009375.D
Acq On : 23 Mar 2019 05:44
Operator : SY/VA
Sample : K2031-19
Misc : 3.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5S9

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:48 AM

Quant Time: Mar 23 06:21:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

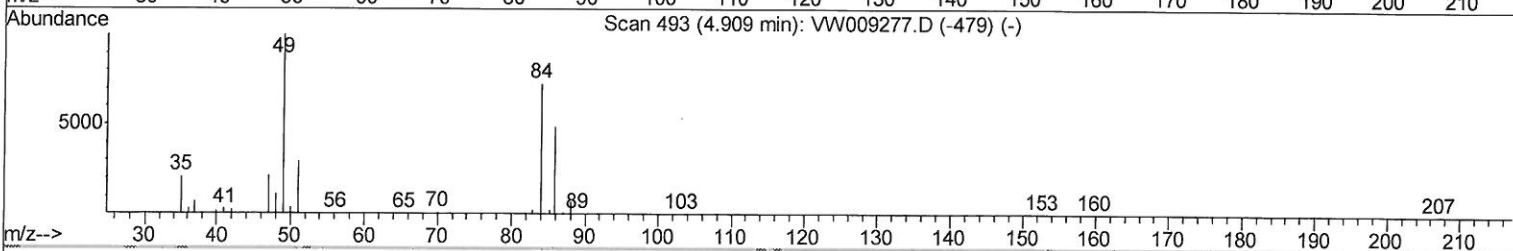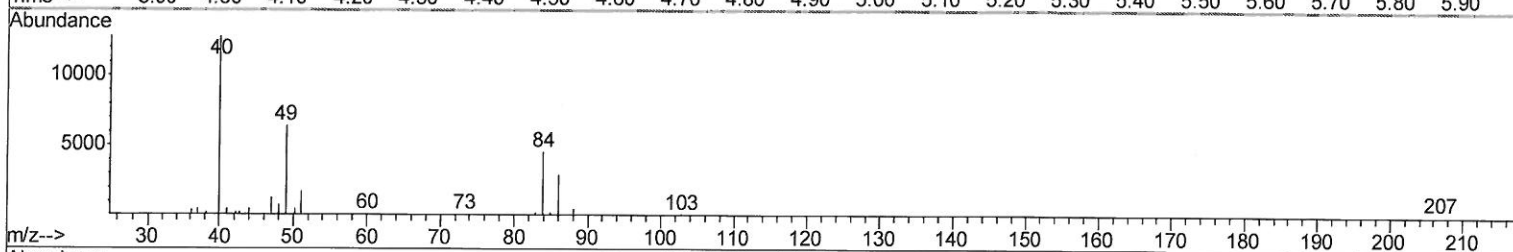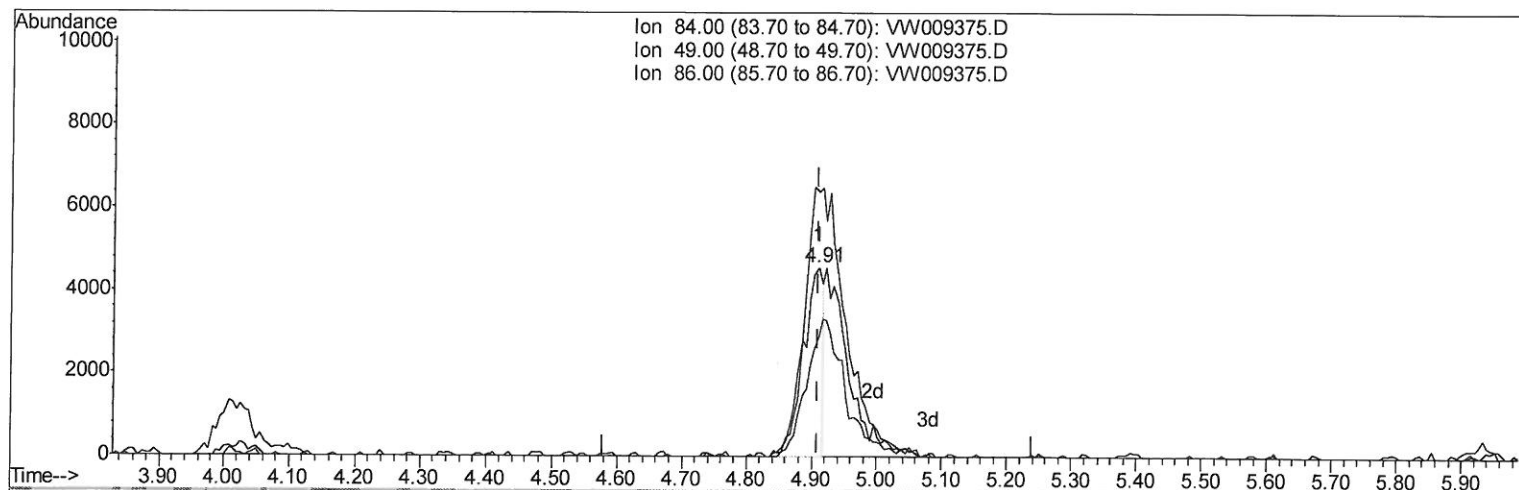

TIC: VW009375.D

(16) Methylene chloride (T)

4.909min (+0.000) 2.52ug/L

response 9450

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	140.35
86.00	63.50	63.52
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009375.D
Acq On : 23 Mar 2019 05:44
Operator : SY/VA
Sample : K2031-19
Misc : 3.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF5S9

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:48 AM

Quant Time: Mar 23 06:21:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

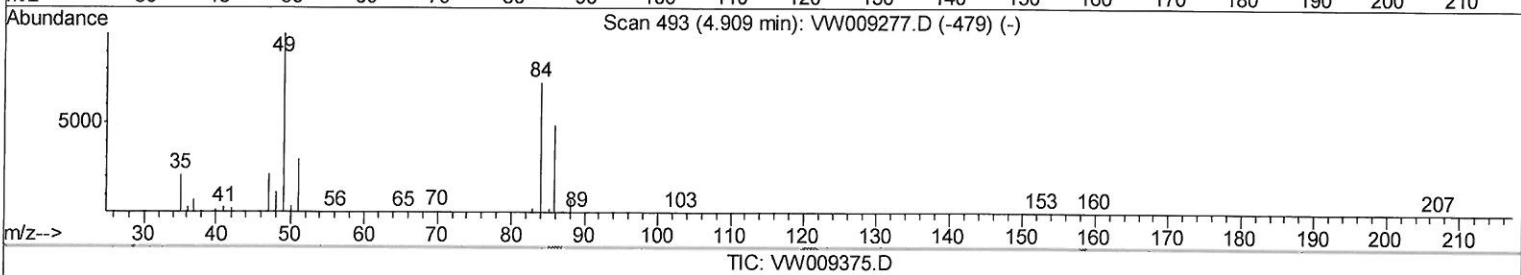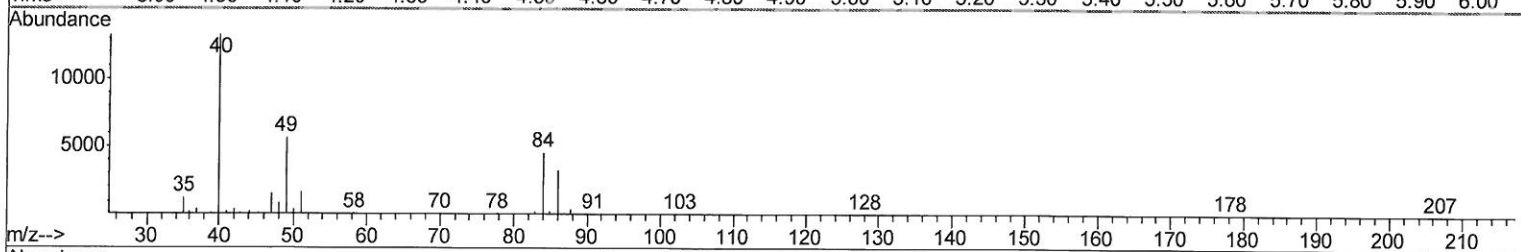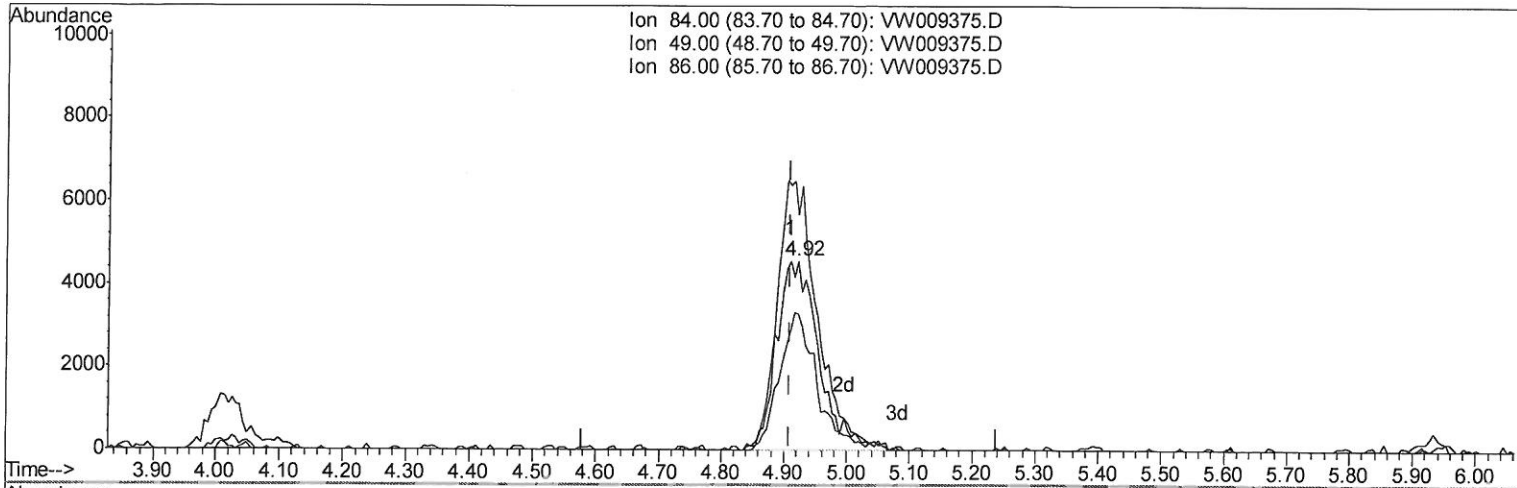

TIC: VW009375.D

(16) Methylene chloride (T)

4.922min (+0.012) 5.62ug/L m

response 21063

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	124.23
86.00	63.50	72.18
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)

Data File : VW009375.D
Acq On : 23 Mar 2019 05:44
Operator : SY/VA
Sample : K2031-19
Misc : 3.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5S9

Quant Time: Mar 23 06:45:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:48 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	256911	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	204885	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	61919	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	85361	27.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.20%
7) Chloroethane-d5	2.90	69	84729	23.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.36%
10) 1,1-Dichloroethene-d2	4.01	63	122402	18.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.80%
20) 2-Butanone-d5	7.08	46	73507	57.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.80%
24) Chloroform-d	7.65	84	187988	26.81	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.24%
26) 1,2-Dichloroethane-d4	8.31	65	115827	27.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.68%
29) Benzene-d6	8.27	84	324798	28.75	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.00%
33) 1,2-Dichloropropane-d6	9.27	67	101656	29.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	119.80%
37) Toluene-d8	10.32	98	243740	23.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.32%
38) trans-1,3-Dichloropropene-	10.58	79	25424	14.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.68%
39) 2-Hexanone-d5	10.93	63	45994	55.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	74643	22.33	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.32%
61) 1,2-Dichlorobenzene-d4	13.86	152	59903	25.23	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.92%

Target Compounds

					Qvalue
13) Acetone	4.13	43	5948	5.713 ug/L	58
14) Carbon disulfide	4.38	76	22293	2.618 ug/L	# 87
16) Methylene chloride	4.92	84	21063m	5.622 ug/L	82/24/1984

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)
Data File : VW009375.D
Acq On : 23 Mar 2019 05:44
Operator : SY/VA
Sample : K2031-19
Misc : 3.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5S9

Quant Time: Mar 23 06:45:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:48 AM

