

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009376.D
Acq On : 23 Mar 2019 06:11
Operator : SY/VA
Sample : K2031-20
Misc : 6.24G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5T0

Quant Time: Mar 23 06:46:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:49 AM

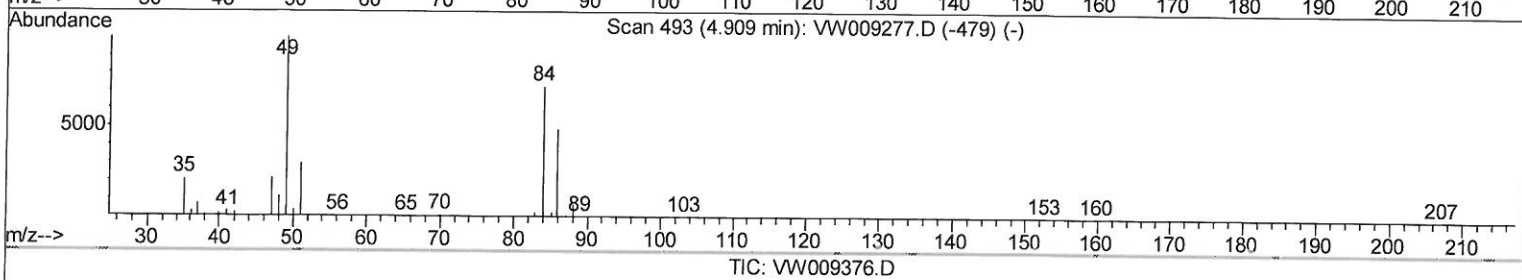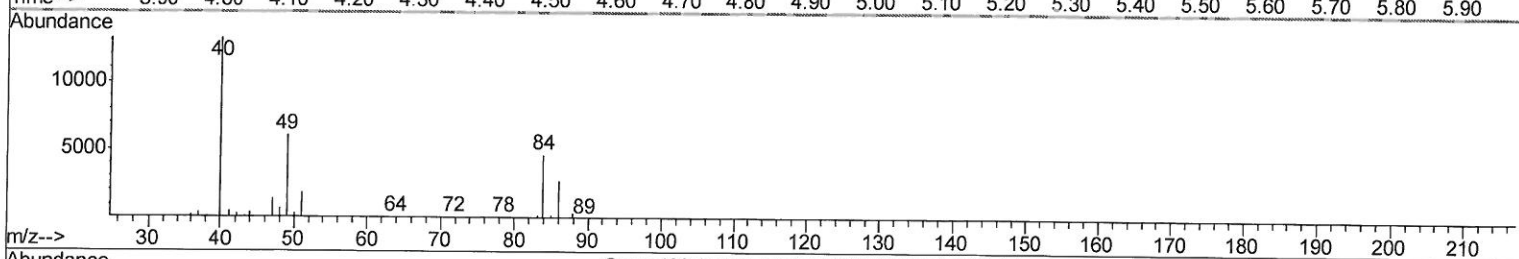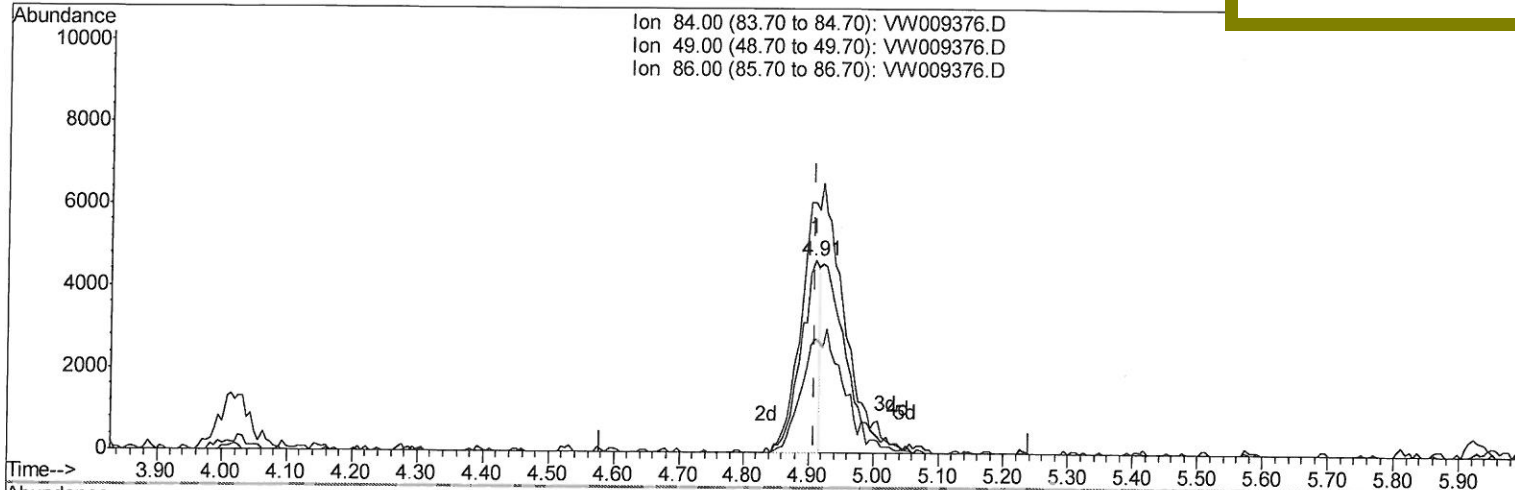

TIC: VW009376.D

(16) Methylene chloride (T)

4.909min (-0.000) 2.21ug/L

response 9494

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	129.87
86.00	63.50	59.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (Qedit)




Data File : VW009376.D
Acq On : 23 Mar 2019 06:11
Operator : SY/VA
Sample : K2031-20
Misc : 6.24G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5T0

Quant Time: Mar 23 06:46:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:49 AM

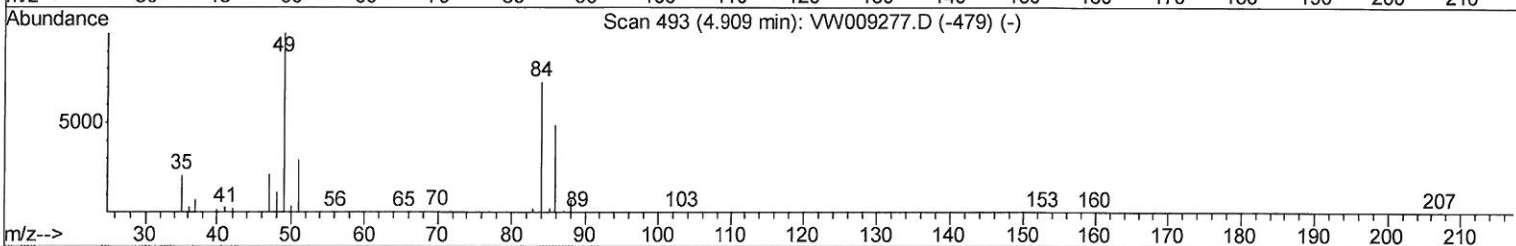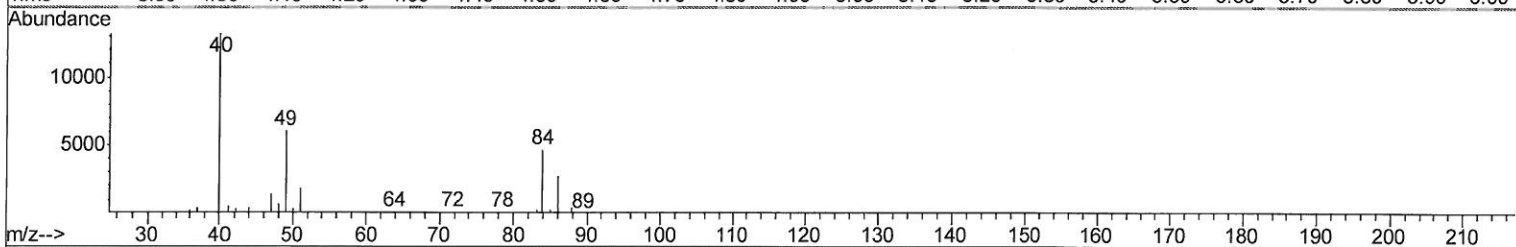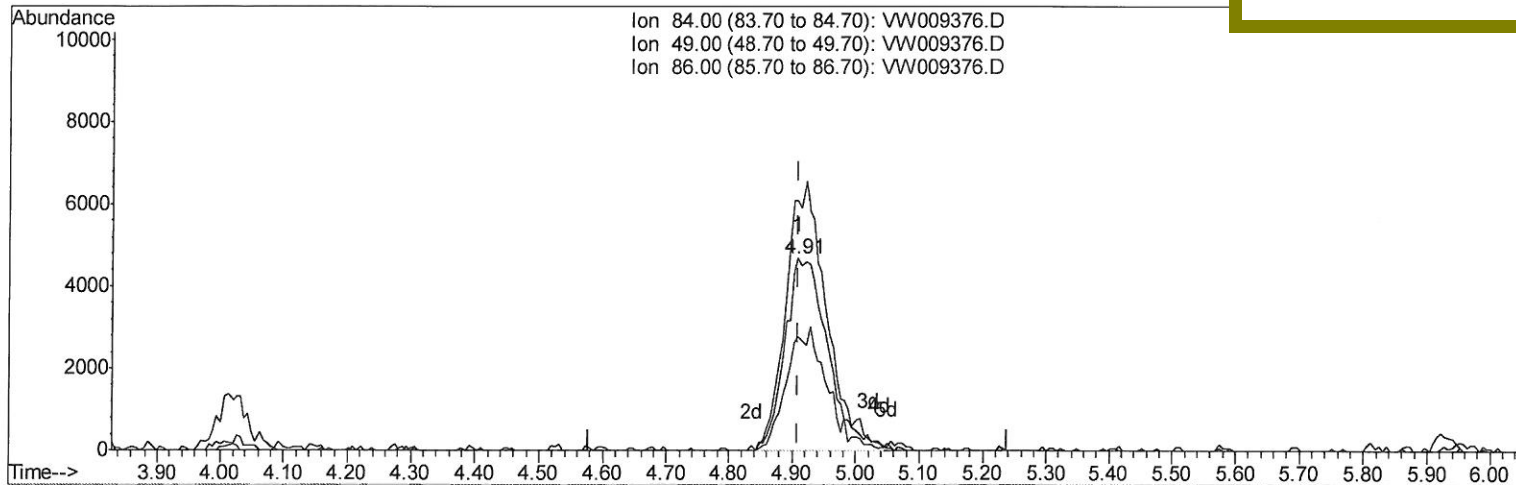

TIC: VW009376.D

(16) Methylene chloride (T)

4.909min (-0.000) 5.09ug/L m

CO 124/19 64

response 21894

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	129.87
86.00	63.50	59.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)

Data File : VW009376.D
Acq On : 23 Mar 2019 06:11
Operator : SY/VA
Sample : K2031-20
Misc : 6.24G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5T0

Quant Time: Mar 23 06:48:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:49 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	295127	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	227484	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	64393	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	74469	21.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.48%
7) Chloroethane-d5	2.89	69	80995	19.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.52%
10) 1,1-Dichloroethene-d2	4.01	63	117240	15.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.52%
20) 2-Butanone-d5	7.08	46	70015	48.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.00%
24) Chloroform-d	7.65	84	191870	23.82	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.28%
26) 1,2-Dichloroethane-d4	8.31	65	128676	26.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.08%
29) Benzene-d6	8.27	84	326813	26.05	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.20%
33) 1,2-Dichloropropane-d6	9.27	67	110306	29.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	117.08%
37) Toluene-d8	10.32	98	244351	21.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.24%
38) trans-1,3-Dichloropropene-	10.58	79	38480	20.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.32%
39) 2-Hexanone-d5	10.93	63	43768	47.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	96194	25.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.68%
61) 1,2-Dichlorobenzene-d4	13.86	152	57694	23.37	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.48%

Target Compounds

				Qvalue
13) Acetone	4.12	43	44751	37.415 ug/L 99
14) Carbon disulfide	4.39	76	10440	1.067 ug/L # 85
16) Methylene chloride	4.91	84	21894m	5.087 ug/L 85
21) 2-Butanone	7.17	43	16635	10.073 ug/L 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032219\
Quantitation Report (QT Reviewed)

Data File : VW009376.D
Acq On : 23 Mar 2019 06:11
Operator : SY/VA
Sample : K2031-20
Misc : 6.24G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5T0

Manual Integrations
APPROVED

MMDadoda
3/25/2019 8:29:49 AM

Quant Time: Mar 23 06:48:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 01:25:26 2019
Response via : Initial Calibration

