

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032219\
 Data File : VW009349.D
 Acq On : 22 Mar 2019 15:32
 Operator : SY/VA
 Sample : K2017-14
 Misc : 4.78G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0E0

Quant Time: Mar 23 00:55:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 23 00:14:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	353362	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	329949	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	143469	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	86082	20.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.56%
7) Chloroethane-d5	2.89	69	86731	17.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.20%
10) 1,1-Dichloroethene-d2	4.01	63	137586	15.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.32%
20) 2-Butanone-d5	7.08	46	60202	34.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.94%
24) Chloroform-d	7.64	84	207168	21.48	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.92%
26) 1,2-Dichloroethane-d4	8.30	65	122521	21.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.36%
29) Benzene-d6	8.27	84	374445	20.58	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.32%
33) 1,2-Dichloropropane-d6	9.27	67	118237	21.63	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.52%
37) Toluene-d8	10.32	98	319817	19.01	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.04%
38) trans-1,3-Dichloropropene-	10.57	79	48998	17.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.40%
39) 2-Hexanone-d5	10.93	63	42059	31.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.54%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	103198	19.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.68%
61) 1,2-Dichlorobenzene-d4	13.86	152	114959	20.90	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.60%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	19126	3.712 ug/L	90
22) cis-1,2-Dichloroethene	7.17	96	83380	16.824 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032219\
Data File : VW009349.D
Acq On : 22 Mar 2019 15:32
Operator : SY/VA
Sample : K2017-14
Misc : 4.78G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0E0

Quant Time: Mar 23 00:55:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 23 00:14:14 2019
Response via : Initial Calibration

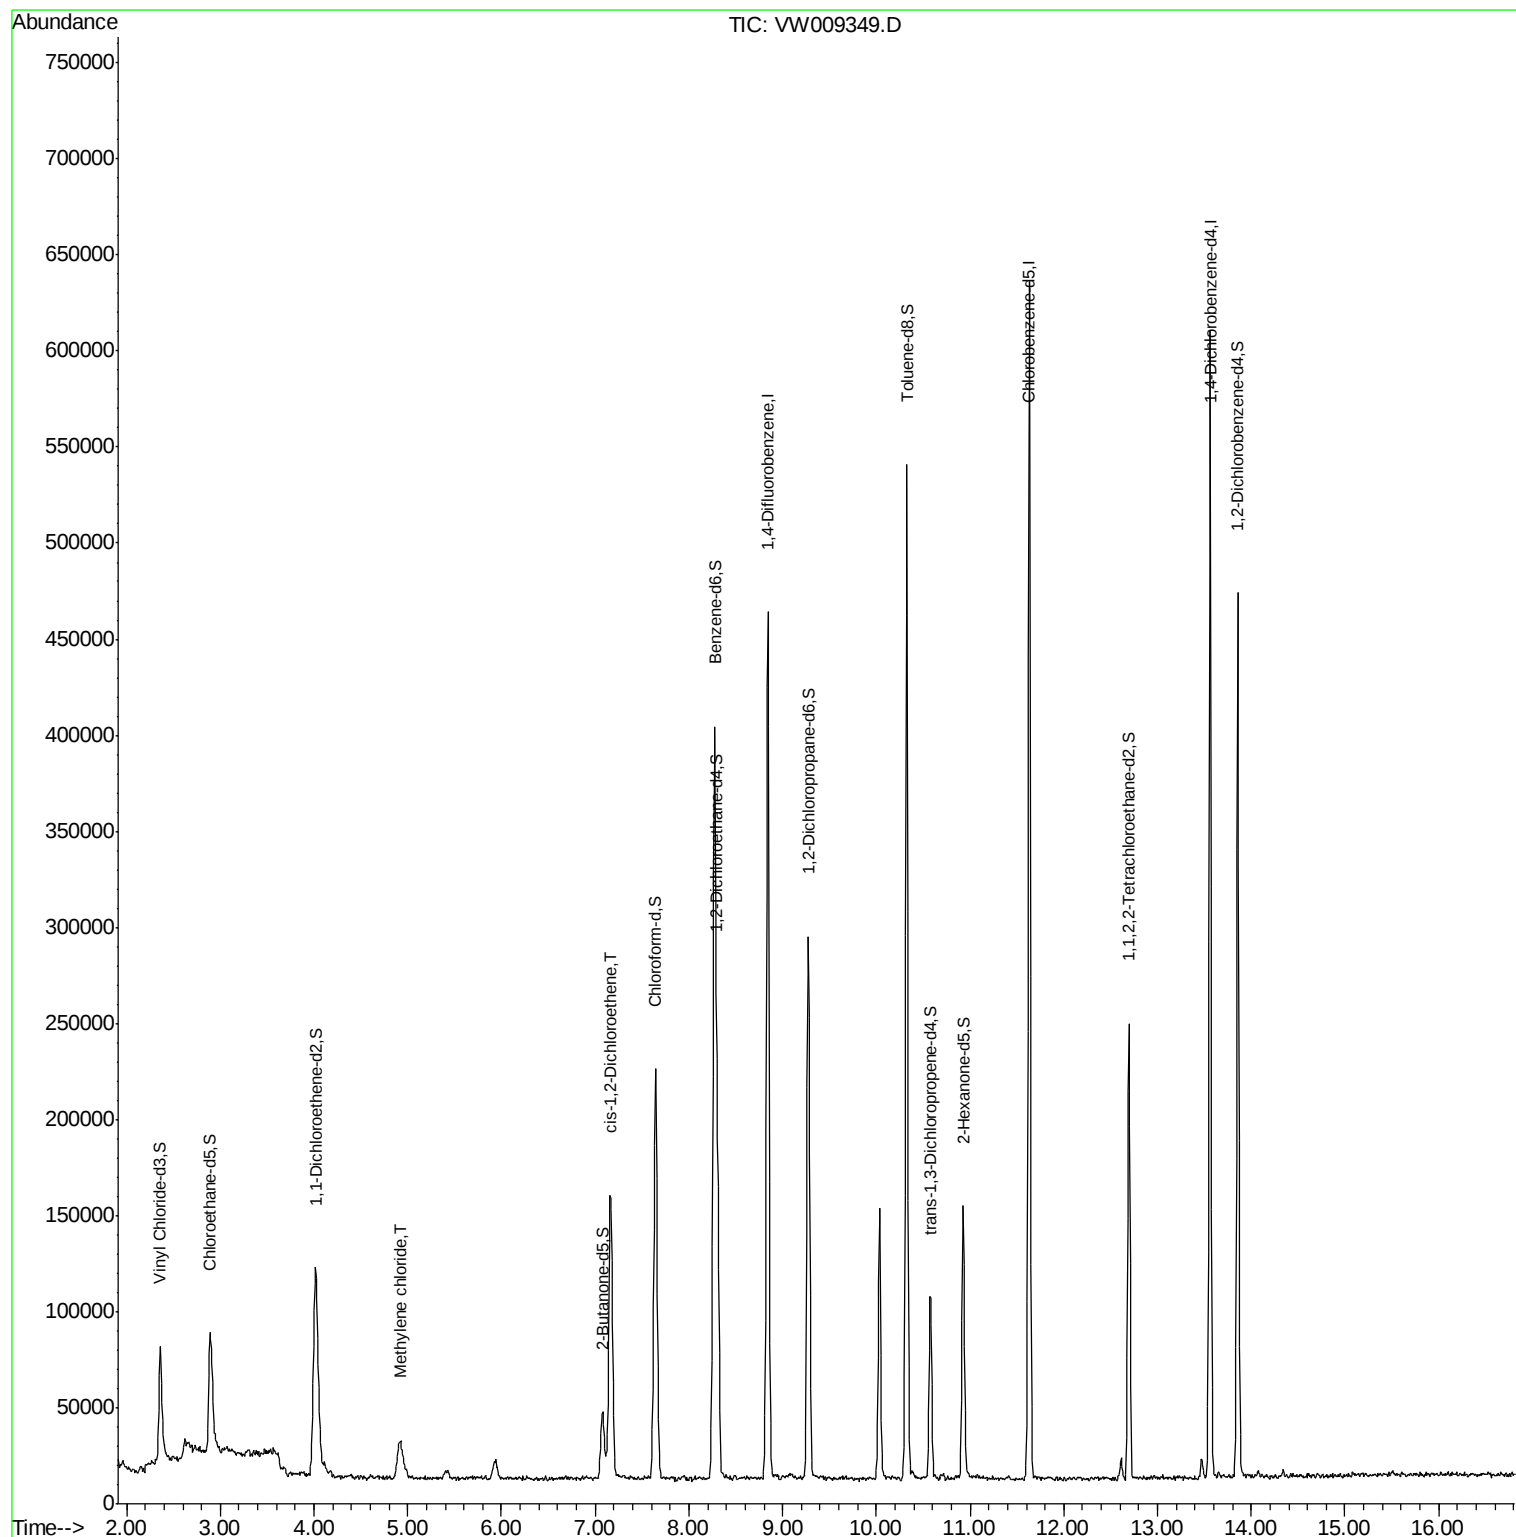


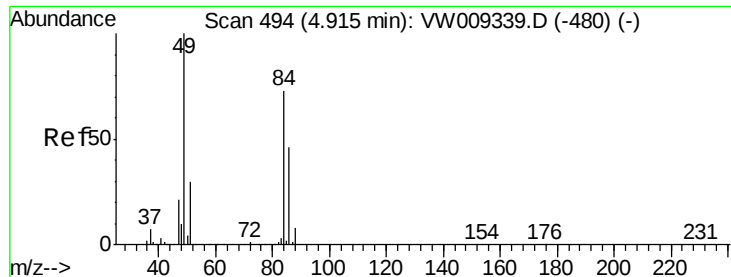




#16
Methylene chloride
Concen: 3.712 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.00 min
Lab File: VW009349.D
Acq: 22 Mar 2019 15:32

Instrument :
MSVOA_W
ClientSampled :
BF0E0

Tot Ion: 84 Resp: 19126
Ion Ratio Lower Upper
84 100
49 123.9 96.0 178.2
86 57.7 44.4 82.5

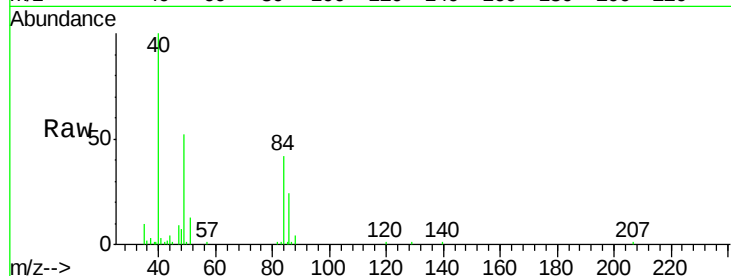


Abundance Ion 84.00 (83.70 to 84.70): VW
Ion 49.00 (48.70 to 49.70): VW
Ion 86.00 (85.70 to 86.70): VW

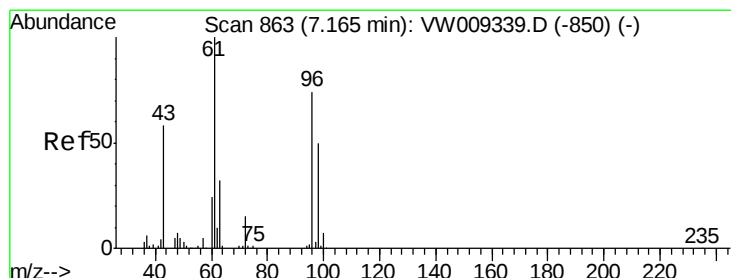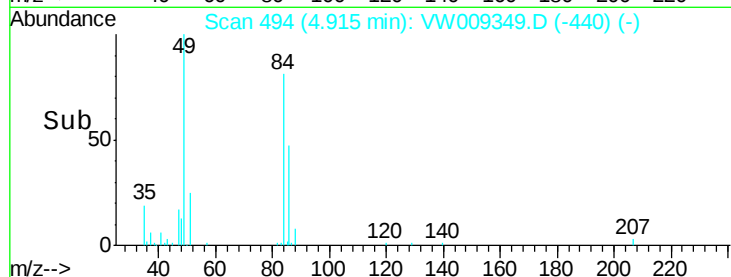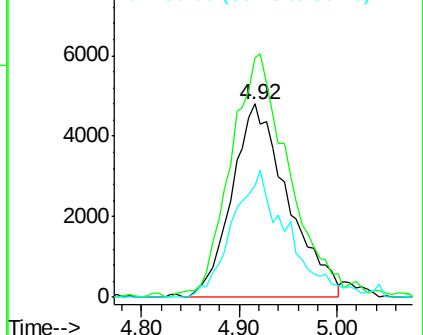

#22
cis-1,2-Dichloroethene
Concen: 16.824 ug/L
RT: 7.17 min Scan# 863
Delta R.T. 0.00 min
Lab File: VW009349.D
Acq: 22 Mar 2019 15:32

Tgt Ion: 96 Resp: 83380
Ion Ratio Lower Upper
96 100
61 122.2 90.6 168.3
98 61.5 44.0 81.8

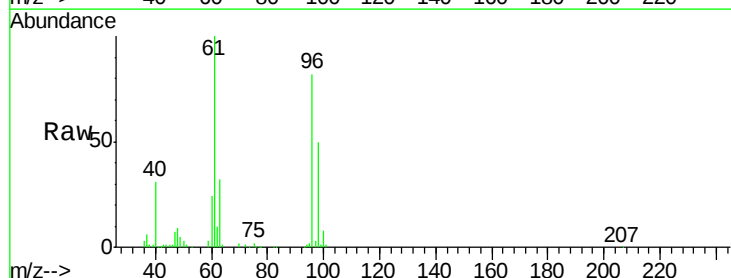

Abundance Ion 96.00 (95.70 to 96.70): VW
Ion 61.00 (60.70 to 61.70): VW
Ion 98.00 (97.70 to 98.70): VW

