


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
Data File : VW018421.D
Acq On : 23 Mar 2021 09:51
Operator : SY/VA
Sample : VW0323SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Manual Integrations
APPROVED

SAM
3/26/2021 6:06:53 PM

Quant Time: Mar 24 01:24:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 24 01:23:39 2021
Response via : Initial Calibration

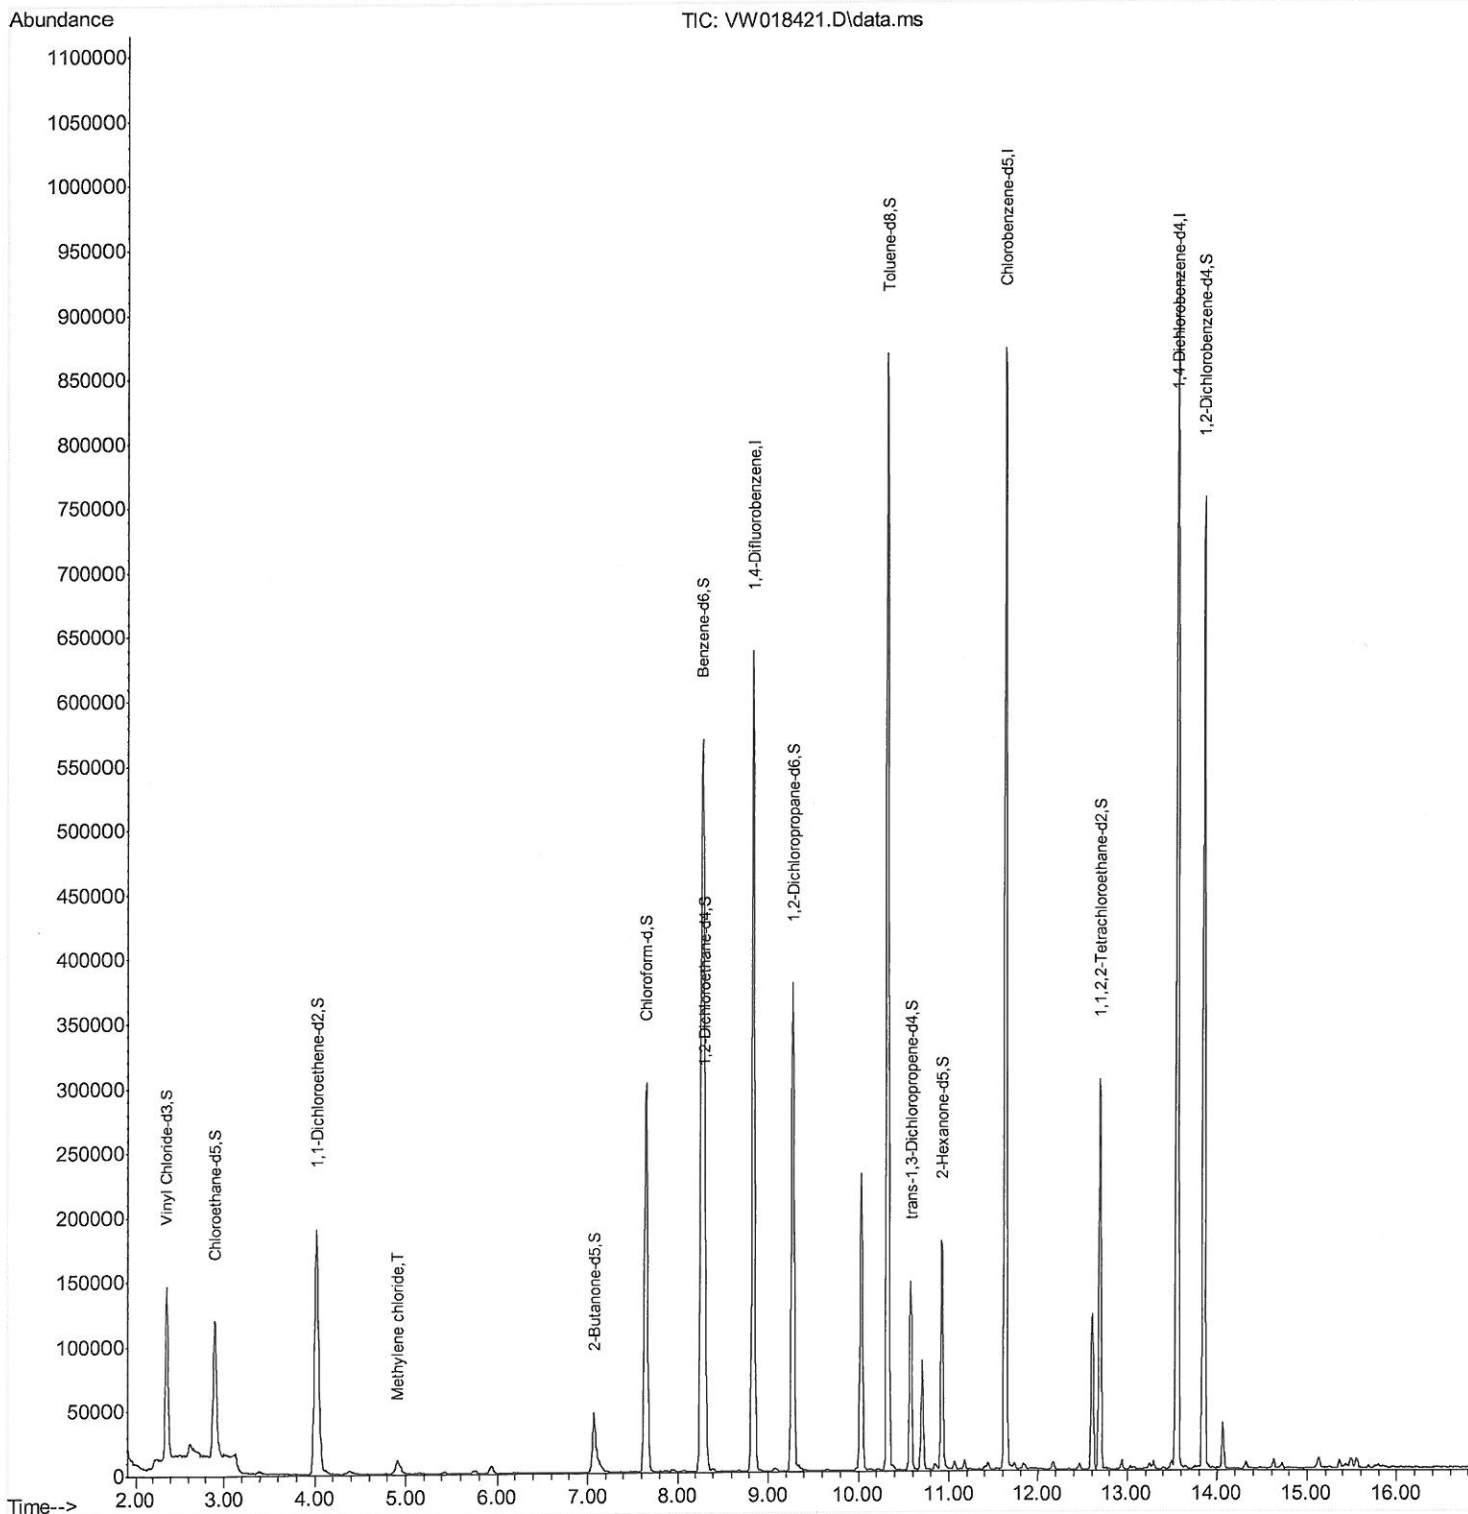

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018421.D
 Acq On : 23 Mar 2021 09:51
 Operator : SY/VA
 Sample : VW0323SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:53 PM

Quant Time: Mar 24 01:24:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

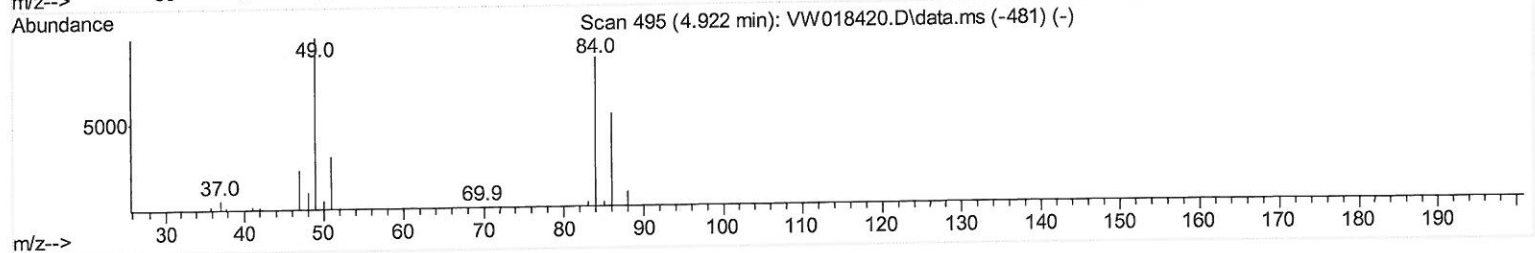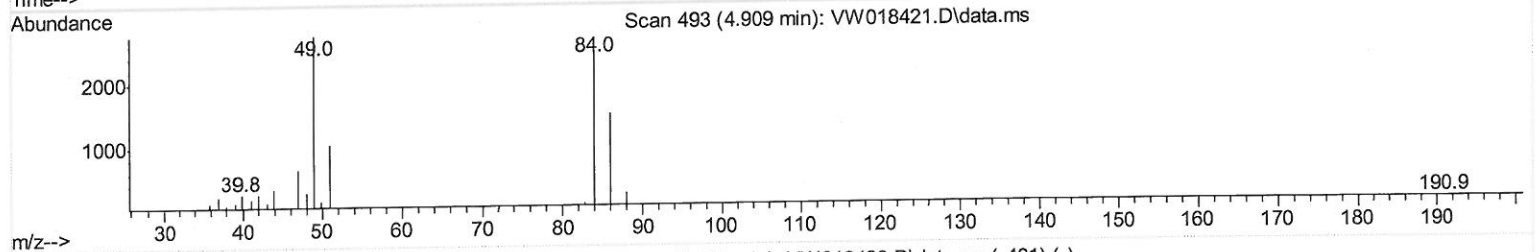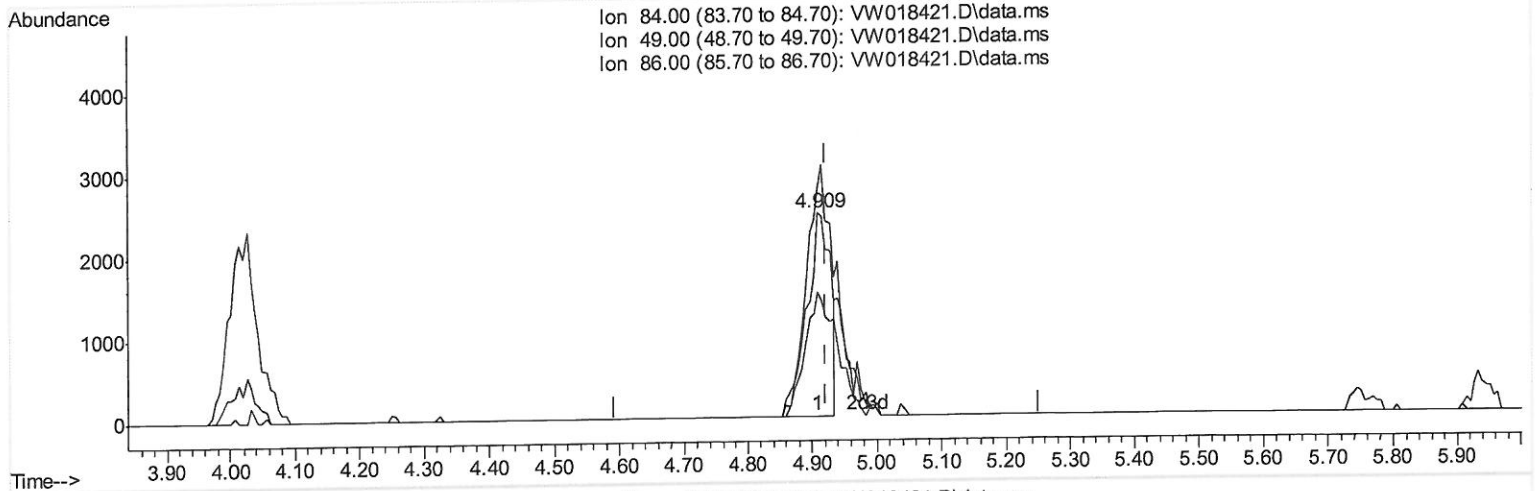

TIC: VW018421.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 0.71 ug/L

response 6136

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	111.32
86.00	65.90	60.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018421.D
 Acq On : 23 Mar 2021 09:51
 Operator : SY/VA
 Sample : VW0323SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:53 PM

Quant Time: Mar 24 01:24:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

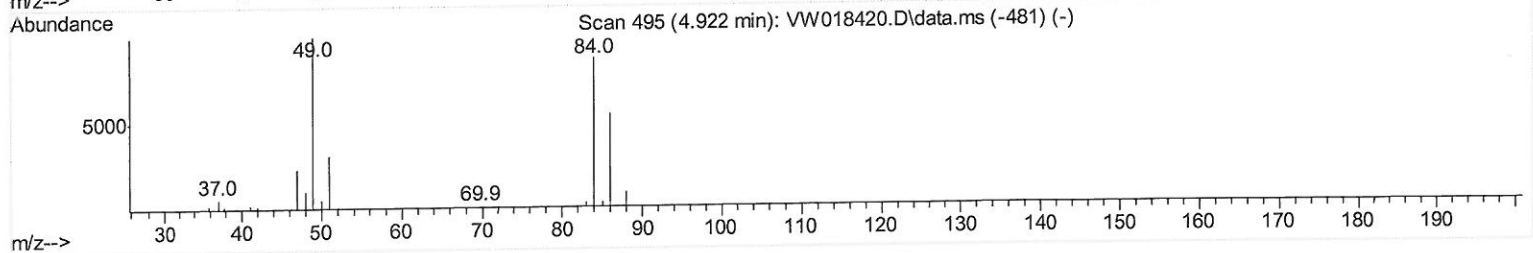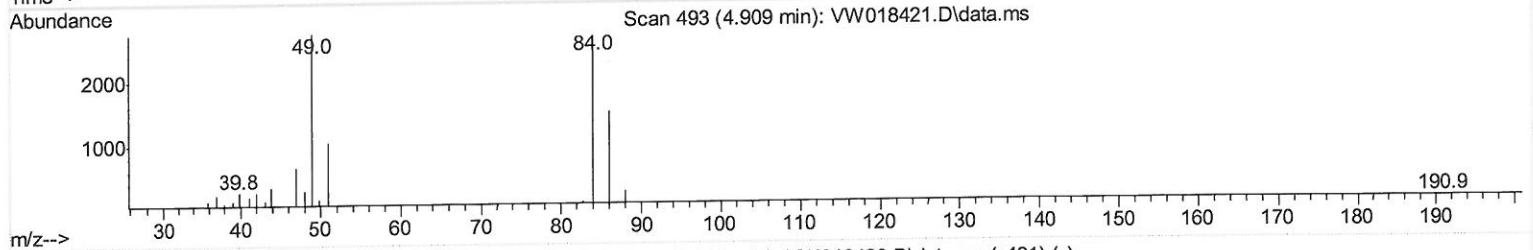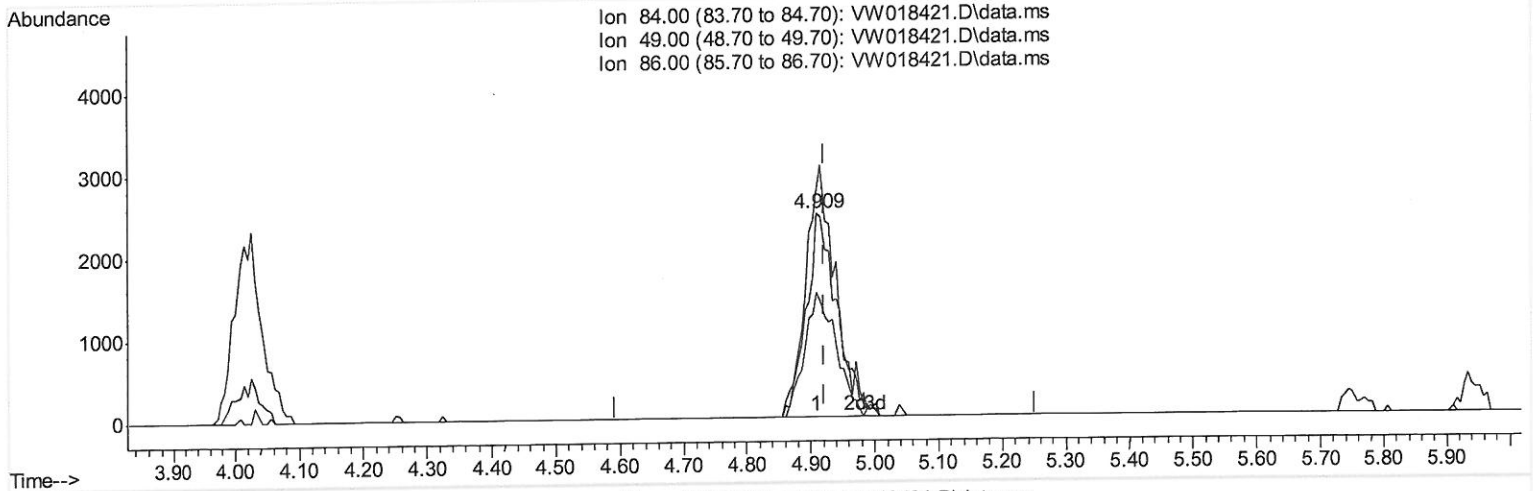

TIC: VW018421.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 0.95 ug/L m

response 8225

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	111.32
86.00	65.90	60.79
0.00	0.00	0.00

7 mo
 3/30/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018421.D
 Acq On : 23 Mar 2021 09:51
 Operator : SY/VA
 Sample : VW0323SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:53 PM

Quant Time: Mar 24 01:24:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	528520	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	474499	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	215215	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	159253	21.65	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	86.60%		
7) Chloroethane-d5	2.892	69	144017	22.37	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	89.48%		
10) 1,1-Dichloroethene-d2	4.019	63	206456	16.26	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	65.04%		
20) 2-Butanone-d5	7.074	46	74796	45.68	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	91.36%		
24) Chloroform-d	7.647	84	299434	22.24	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	88.96%		
26) 1,2-Dichloroethane-d4	8.305	65	179345	22.82	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	91.28%		
29) Benzene-d6	8.275	84	588107	23.31	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	93.24%		
33) 1,2-Dichloropropane-d6	9.275	67	168587	23.17	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	92.68%		
37) Toluene-d8	10.323	98	555079	22.85	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	91.40%		
38) trans-1,3-Dichloroprop...	10.579	79	81437	21.70	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	86.80%		
39) 2-Hexanone-d5	10.921	63	63109	44.32	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	88.64%		
48) 1,1,2,2-Tetrachloroeth...	12.689	84	142800	21.94	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	87.76%		
61) 1,2-Dichlorobenzene-d4	13.853	152	187790	24.54	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	98.16%		

Target Compounds

16) Methylene chloride	4.909	84	8225m	0.95	ug/L	Qvalue
------------------------	-------	----	-------	------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

ML
 3/30/21