


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
Data File : VW018427.D
Acq On : 23 Mar 2021 15:29
Operator : SY/VA
Sample : M1781-06
Misc : 5.73G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4L7

Manual Integrations
APPROVED

SAM
3/26/2021 6:06:33 PM

Quant Time: Mar 24 01:26:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 24 01:23:39 2021
Response via : Initial Calibration

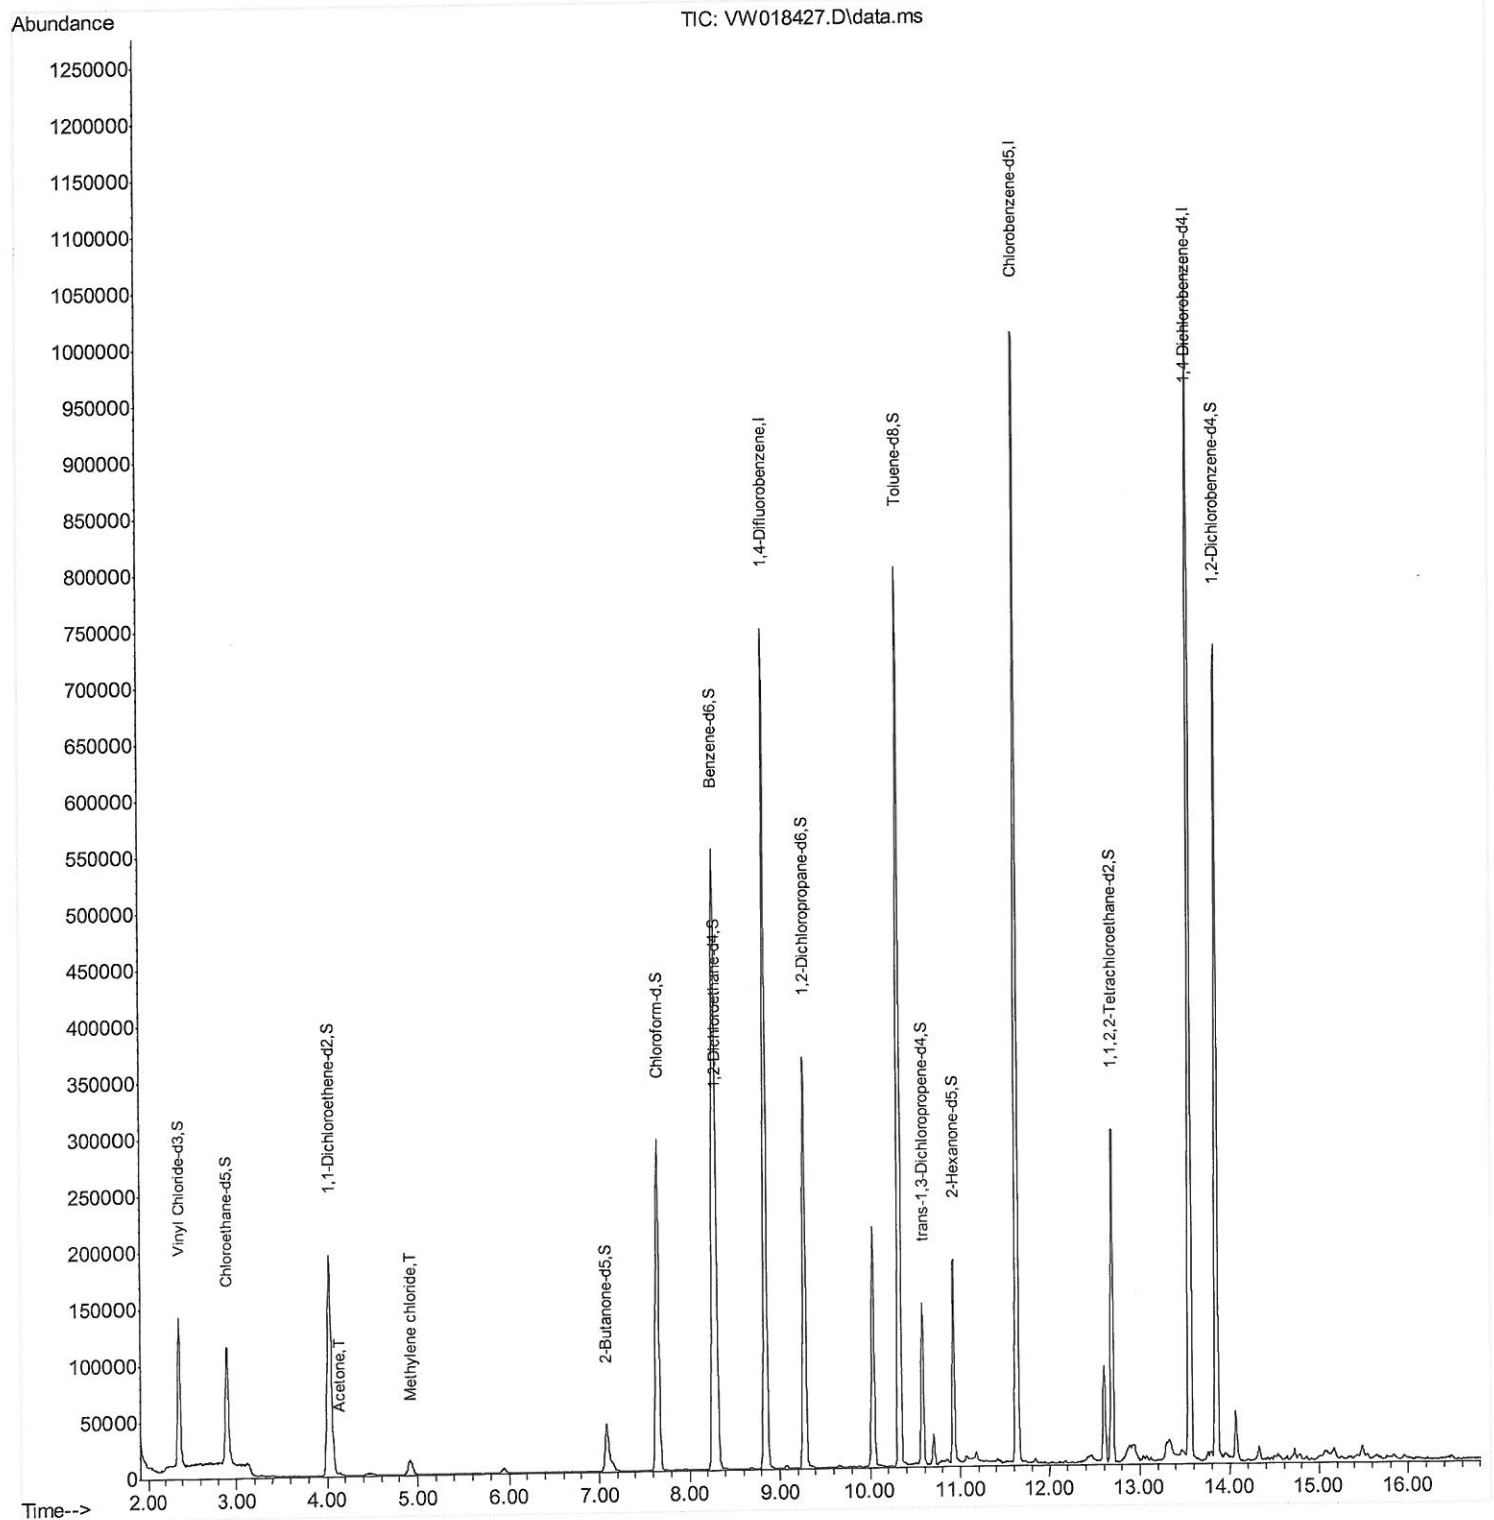

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018427.D
 Acq On : 23 Mar 2021 15:29
 Operator : SY/VA
 Sample : M1781-06
 Misc : 5.73G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4L7

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:33 PM

Quant Time: Mar 24 01:26:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

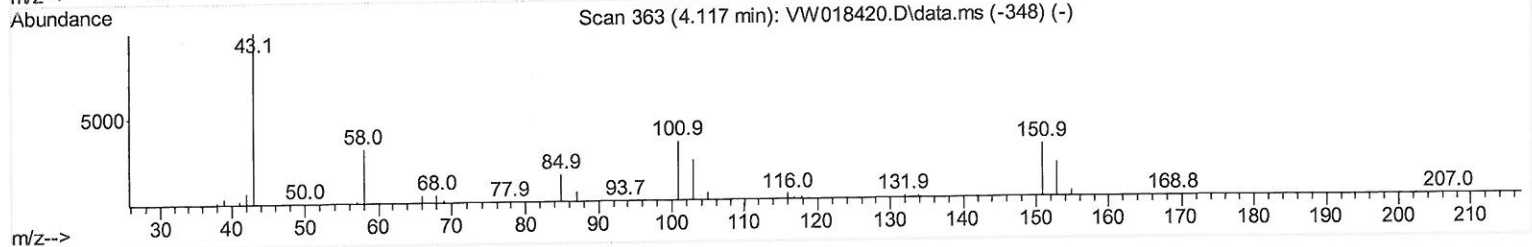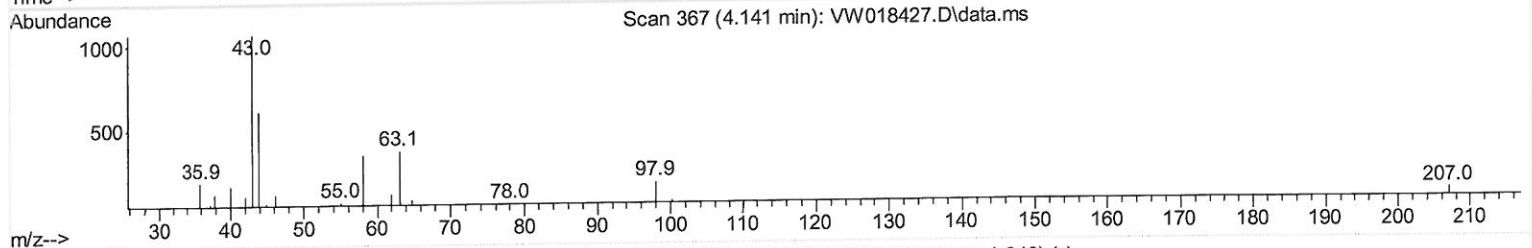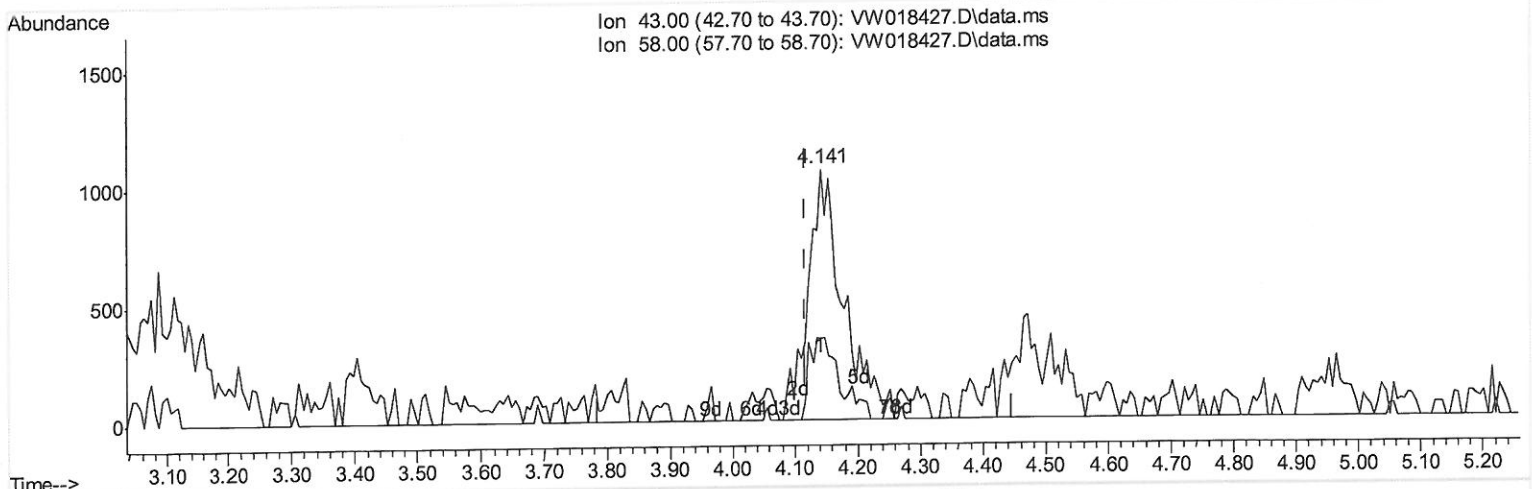

TIC: VW018427.D\data.ms

(13) Acetone (T)

4.141min (+ 0.024) 3.05 ug/L m

response 4137

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	14.07
0.00	0.00	0.00
0.00	0.00	0.00

7 m8
 3/30/21

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018427.D
 Acq On : 23 Mar 2021 15:29
 Operator : SY/VA
 Sample : M1781-06
 Misc : 5.73G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4L7

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:33 PM

Quant Time: Mar 24 01:26:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

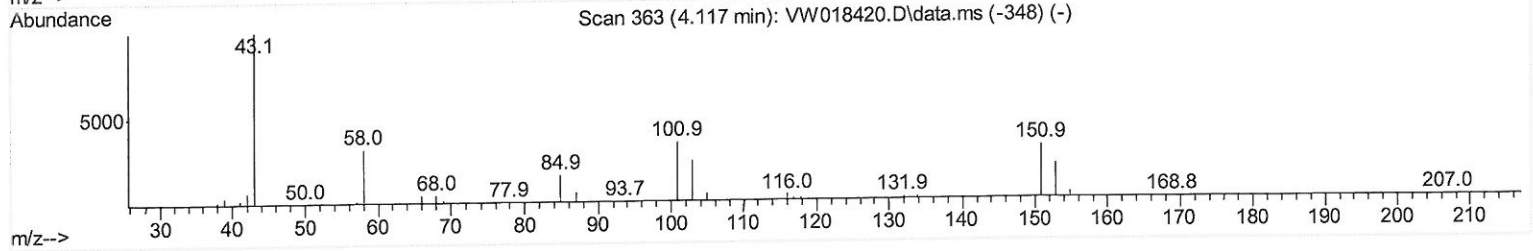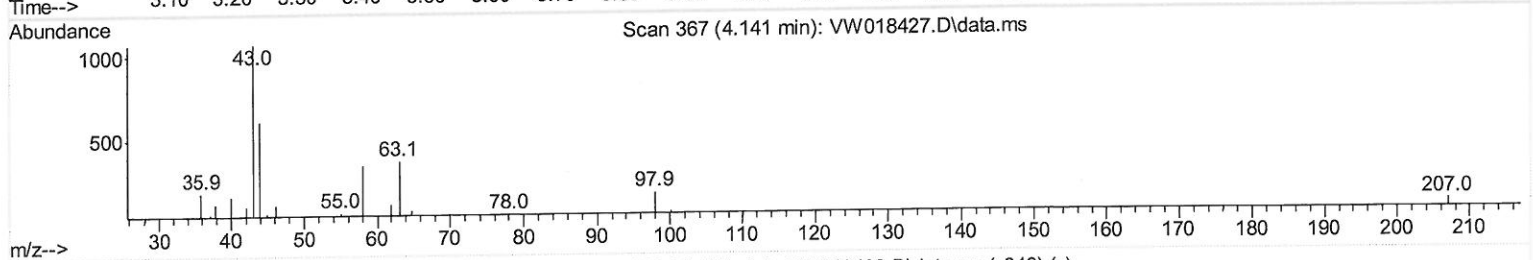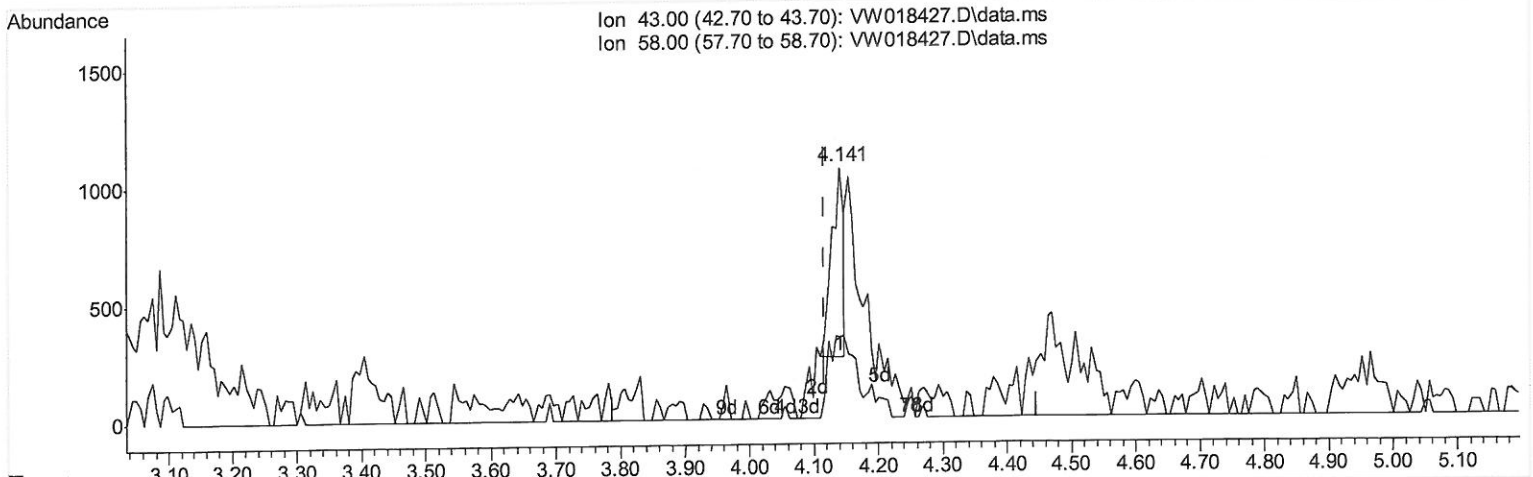

TIC: VW018427.D\data.ms

(13) Acetone (T)

4.141min (+ 0.024) 0.78 ug/L

response 1055

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	55.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032321\
 Data File : VW018427.D
 Acq On : 23 Mar 2021 15:29
 Operator : SY/VA
 Sample : M1781-06
 Misc : 5.73G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG4L7

Manual Integrations
 APPROVED

SAM
 3/26/2021 6:06:33 PM

Quant Time: Mar 24 01:26:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 24 01:23:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	609338	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	551268	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	262103	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	158179	18.65	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	74.60%		
7) Chloroethane-d5	2.898	69	139168	18.75	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	75.00%		
10) 1,1-Dichloroethene-d2	4.019	63	212125	14.49	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	57.96%		
20) 2-Butanone-d5	7.080	46	72279	38.29	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	76.58%		
24) Chloroform-d	7.653	84	292369	18.84	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	75.36%		
26) 1,2-Dichloroethane-d4	8.305	65	177125	19.55	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	78.20%		
29) Benzene-d6	8.275	84	565135	19.28	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	77.12%		
33) 1,2-Dichloropropane-d6	9.274	67	163272	19.31	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	77.24%		
37) Toluene-d8	10.323	98	525595	18.63	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	74.52%		
38) trans-1,3-Dichloroprop...	10.579	79	76435	17.53	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	70.12%		
39) 2-Hexanone-d5	10.927	63	62769	37.94	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	75.88%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	142924	18.90	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	75.60%		
61) 1,2-Dichlorobenzene-d4	13.853	152	178104	19.11	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	76.44%		
Target Compounds						
13) Acetone	4.141	43	4137m	3.05	ug/L	Qvalue
16) Methylene chloride	4.928	84	10879	1.09	ug/L	96

7 m8
 3/30/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed