

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032421\
 Data File : VW018444.D
 Acq On : 24 Mar 2021 15:53
 Operator : SY/VA
 Sample : M1784-14
 Misc : 4.62G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4X6

Quant Time: Mar 25 01:26:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 25 01:23:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	487831	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	438670	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	201761	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	172854	25.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.84%
7) Chloroethane-d5	2.892	69	160443	27.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.00%
10) 1,1-Dichloroethene-d2	4.026	63	199566	17.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.12%
20) 2-Butanone-d5	7.074	46	66886	44.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.52%
24) Chloroform-d	7.647	84	286492	23.06	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.24%
26) 1,2-Dichloroethane-d4	8.305	65	166672	22.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.92%
29) Benzene-d6	8.275	84	556145	23.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.40%
33) 1,2-Dichloropropane-d6	9.275	67	160744	23.90	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.60%
37) Toluene-d8	10.323	98	518509	23.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.36%
38) trans-1,3-Dichloroprop...	10.579	79	68735	19.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.24%
39) 2-Hexanone-d5	10.921	63	56445	42.88	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.76%
48) 1,1,2,2-Tetrachloroeth...	12.689	84	130828	21.74	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.96%
61) 1,2-Dichlorobenzene-d4	13.853	152	170278	23.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.96%
Target Compounds						
16) Methylene chloride	4.922	84	9916	1.24	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032421\
Data File : VW018444.D
Acq On : 24 Mar 2021 15:53
Operator : SY/VA
Sample : M1784-14
Misc : 4.62G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4X6

Quant Time: Mar 25 01:26:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 25 01:23:35 2021
Response via : Initial Calibration

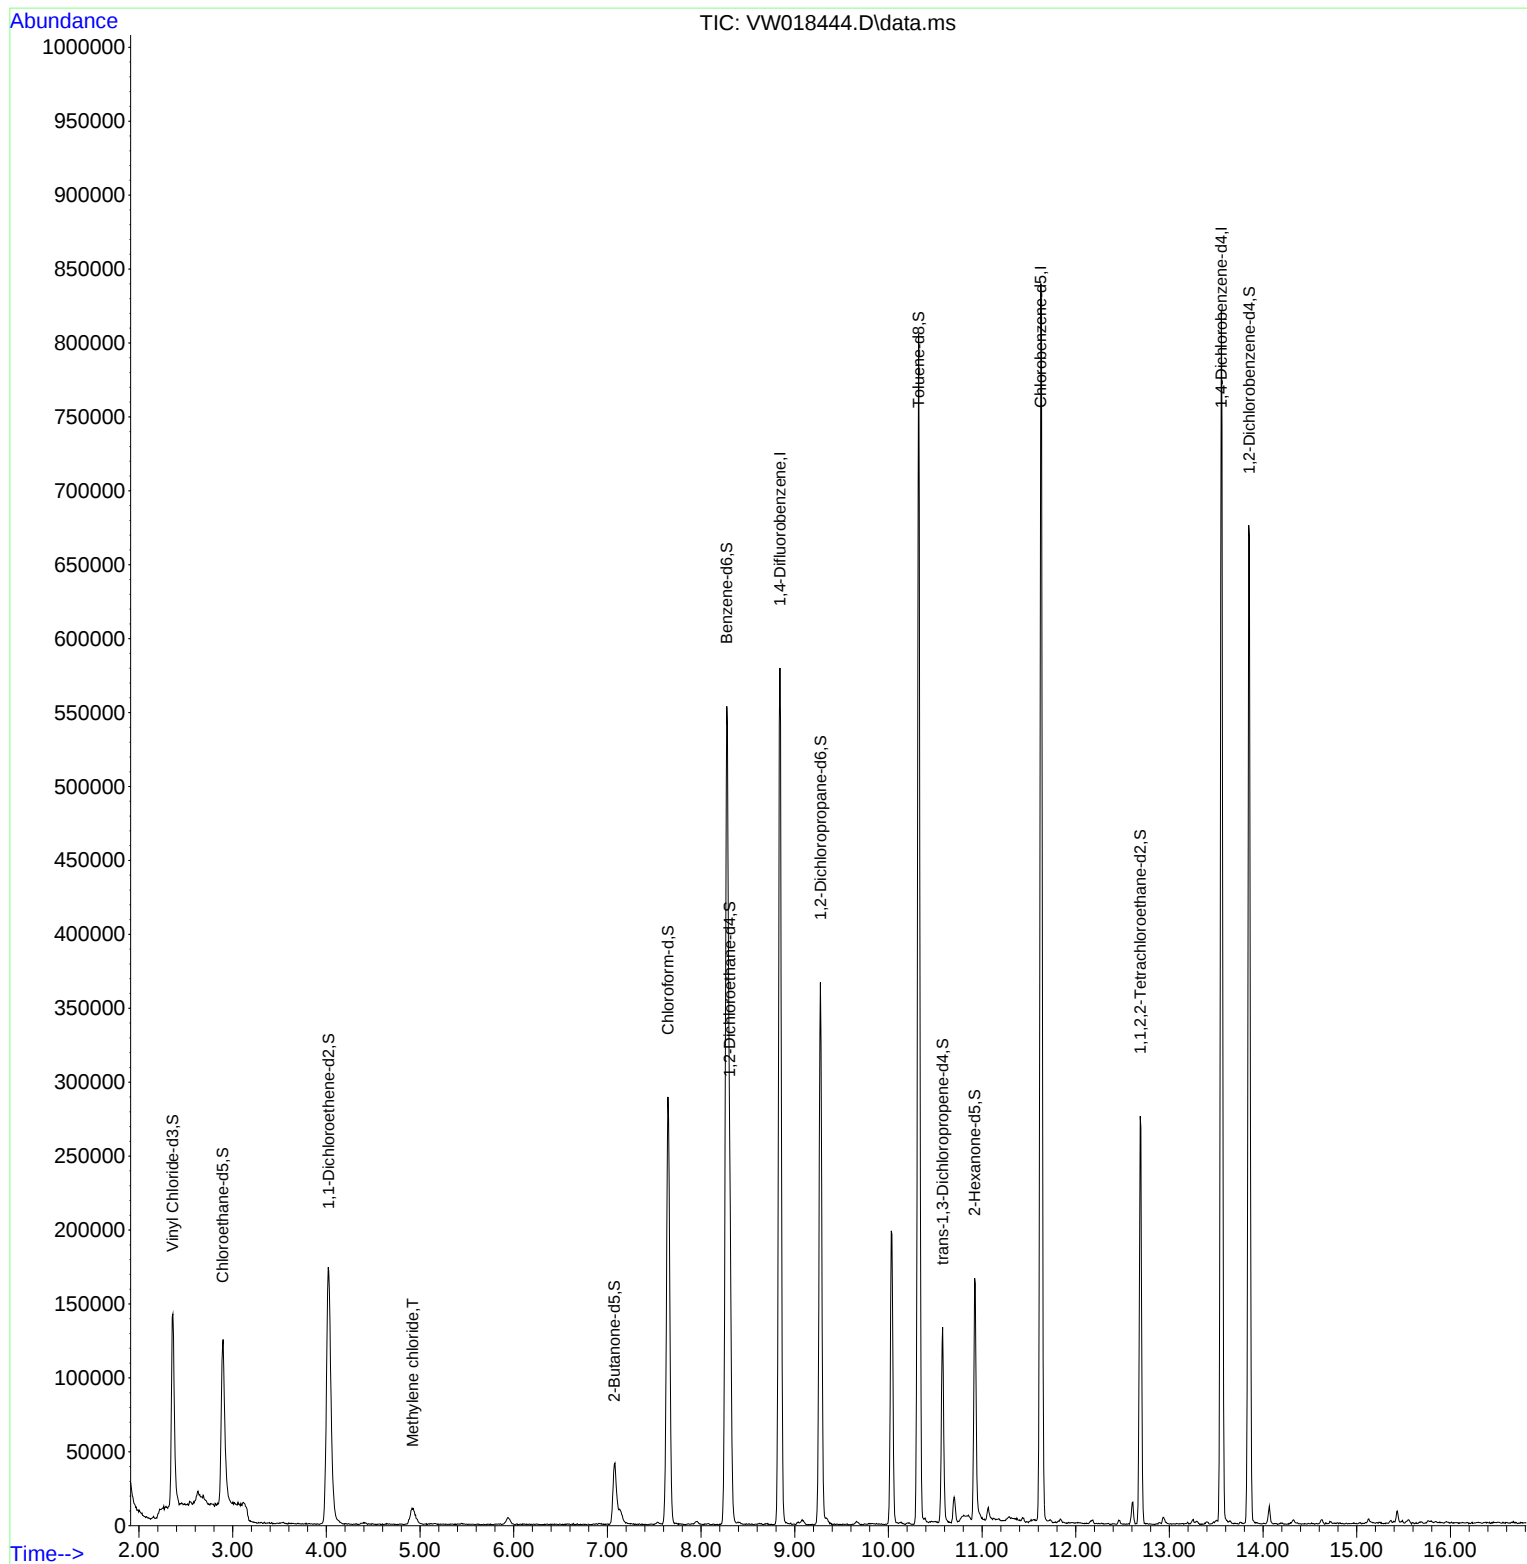

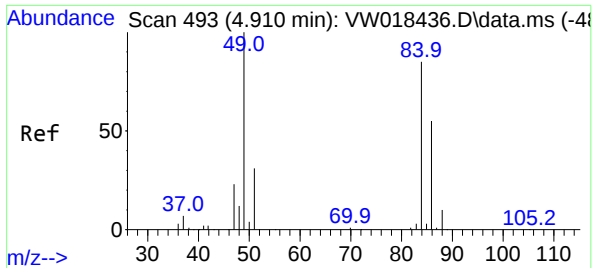

#16
Methylene chloride
Concen: 1.24 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.012 min
Lab File: VW018444.D
Acq: 24 Mar 2021 15:53

Instrument :
MSVOA_W
ClientSampleId :
BG4X6

Tgt Ion: 84 Resp: 9916

Ion	Ratio	Lower	Upper
84	100		
49	99.3	74.4	138.2
86	47.2	46.1	85.7

