
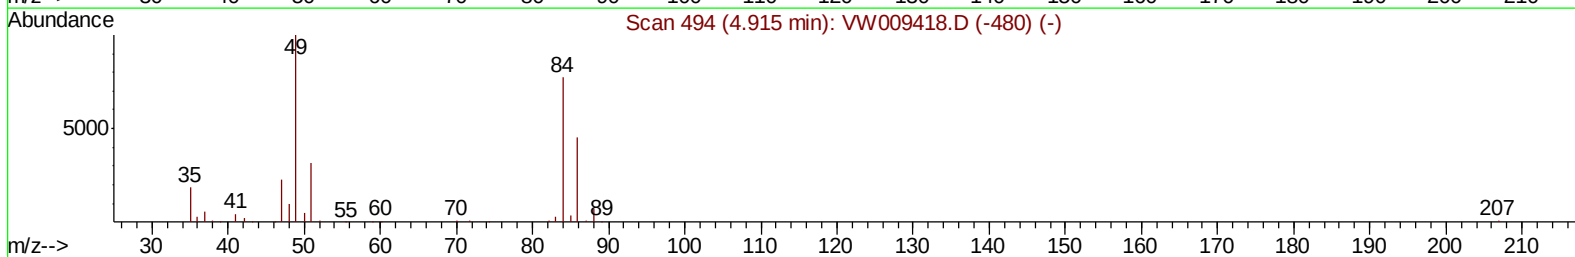
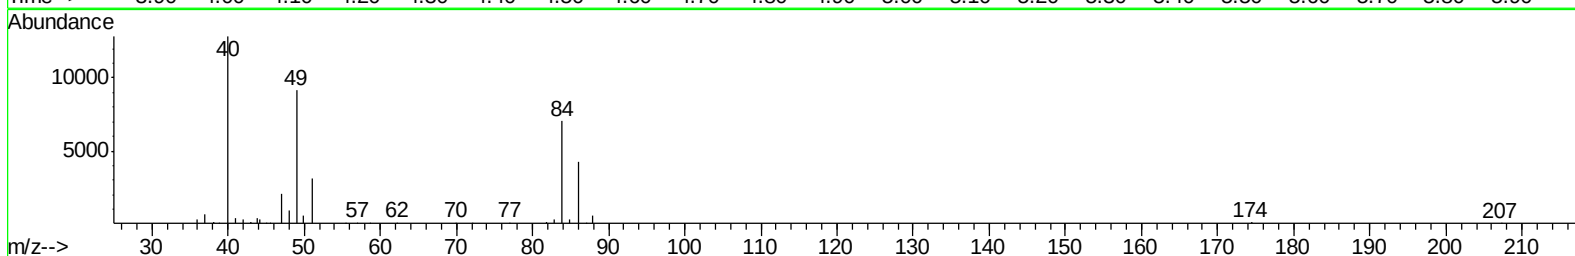


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009429.D
Acq On : 25 Mar 2019 15:41
Operator : SY/VA
Sample : K2031-18
Misc : 4.07G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:51:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

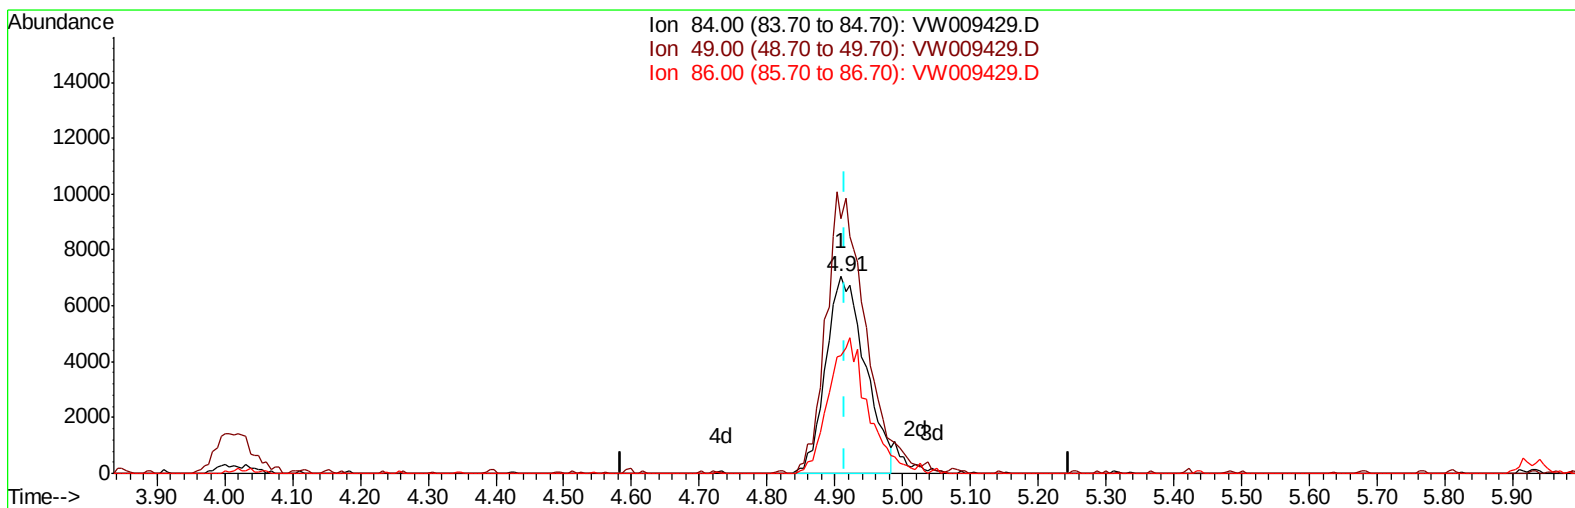

TIC: VW009429.D

(16) Methylene chloride (T)




4.909min (-0.006) 5.26ug/L

response 28535

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	129.36
86.00	63.50	59.90
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009429.D
Acq On : 25 Mar 2019 15:41
Operator : SY/VA
Sample : K2031-18
Misc : 4.07G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:51:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

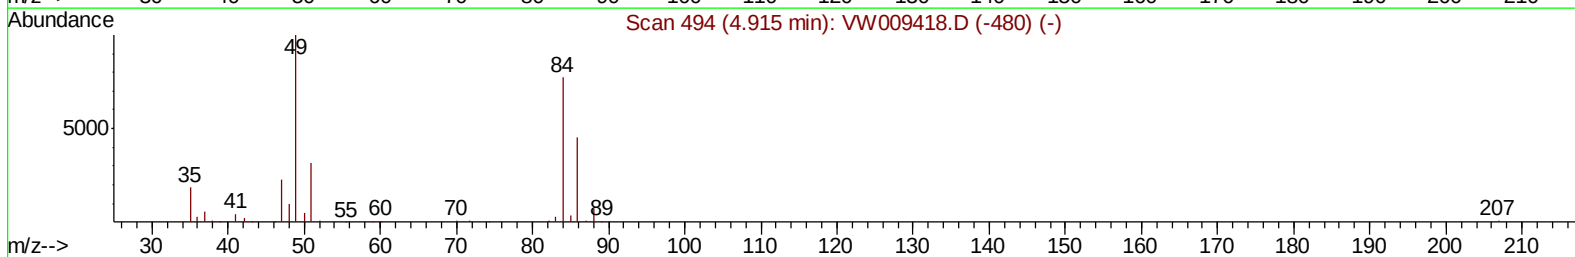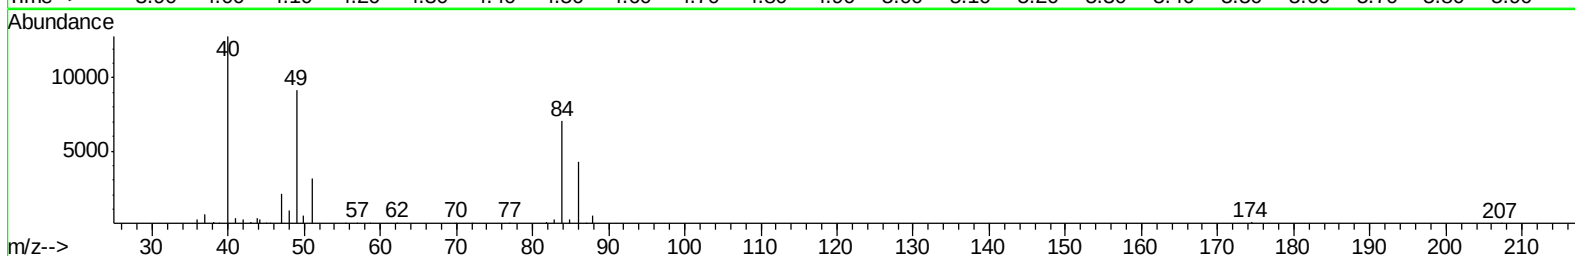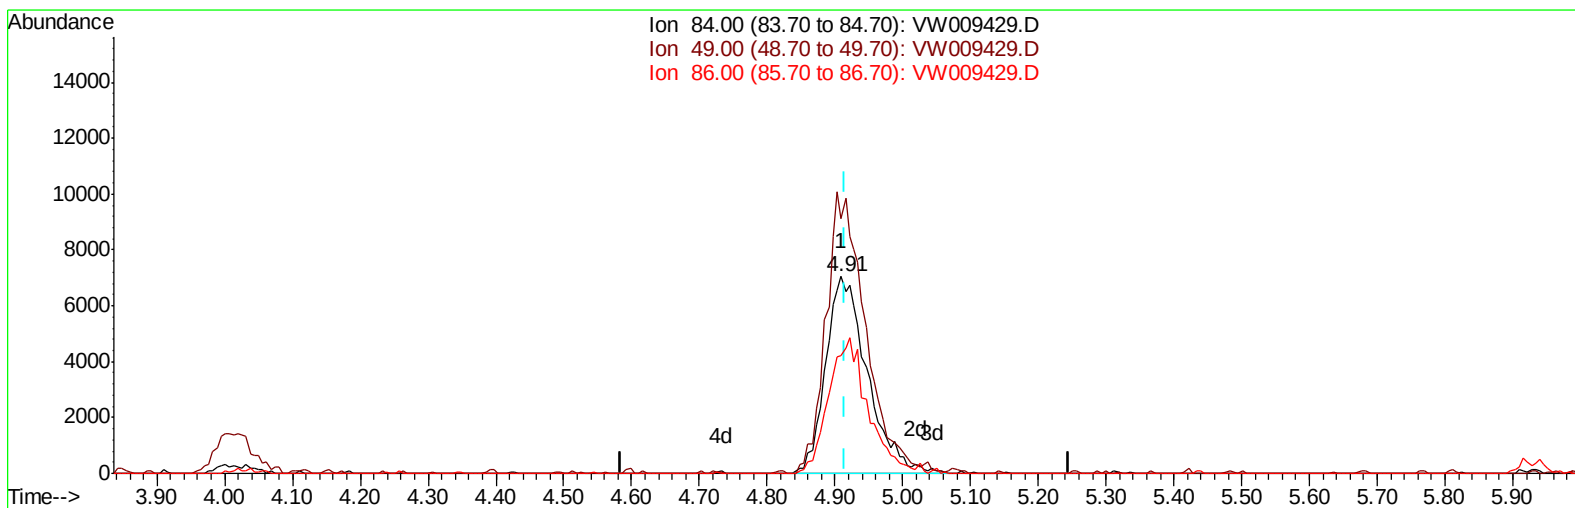

TIC: VW009429.D

(16) Methylene chloride (T)

4.909min (-0.006) 5.26ug/L

response 28535

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	129.36
86.00	63.50	59.90
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009429.D
 Acq On : 25 Mar 2019 15:41
 Operator : SY/VA
 Sample : K2031-18
 Misc : 4.07G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:54:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	371958	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	303387	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	100442	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90278	20.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.24%
7) Chloroethane-d5	2.89	69	103746	19.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.80%
10) 1,1-Dichloroethene-d2	4.01	63	144135	15.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.00%
20) 2-Butanone-d5	7.07	46	85867	46.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.42%
24) Chloroform-d	7.65	84	228999	22.56	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.24%
26) 1,2-Dichloroethane-d4	8.31	65	137504	22.49	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.96%
29) Benzene-d6	8.27	84	397830	23.78	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.12%
33) 1,2-Dichloropropane-d6	9.27	67	127635	25.40	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.60%
37) Toluene-d8	10.32	98	322019	20.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.24%
38) trans-1,3-Dichloropropene-	10.58	79	47298	18.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.96%
39) 2-Hexanone-d5	10.93	63	53860	44.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.50%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	101515	20.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	79382	20.61	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.44%

Target Compounds

					Ovalue
13) Acetone	4.12	43	61236	40.622	ug/L 99
14) Carbon disulfide	4.37	76	66573	5.401	ug/L 97
16) Methylene chloride	4.91	84	28535	5.261	ug/L 94
21) 2-Butanone	7.18	43	19019	9.137	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009429.D
Acq On : 25 Mar 2019 15:41
Operator : SY/VA
Sample : K2031-18
Misc : 4.07G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:54:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

