
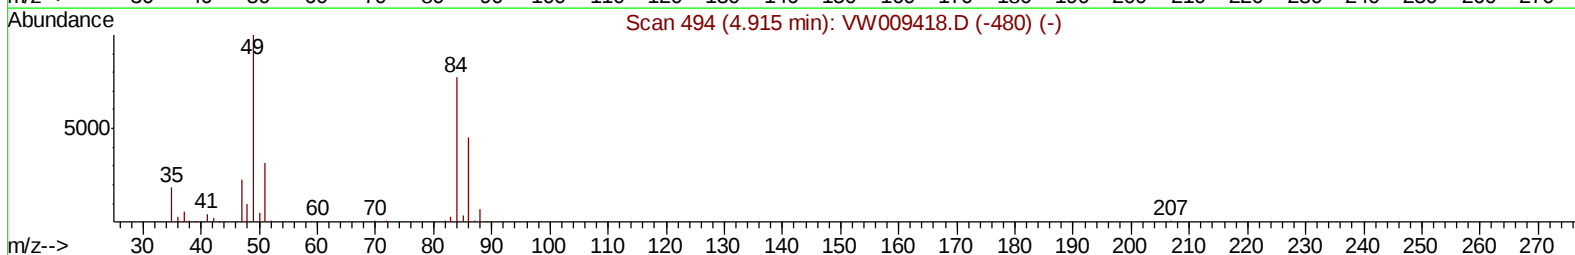
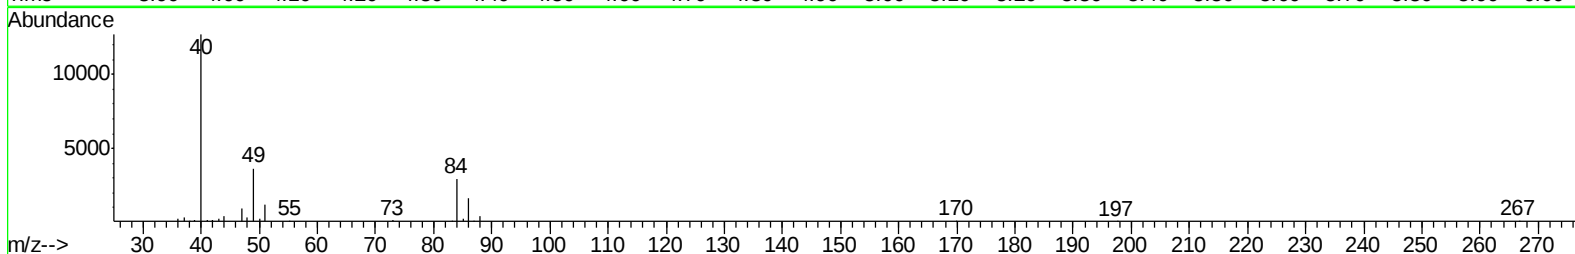


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009421.D
Acq On : 25 Mar 2019 12:02
Operator : SY/VA
Sample : K2062-03
Misc : 5.92G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:50:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

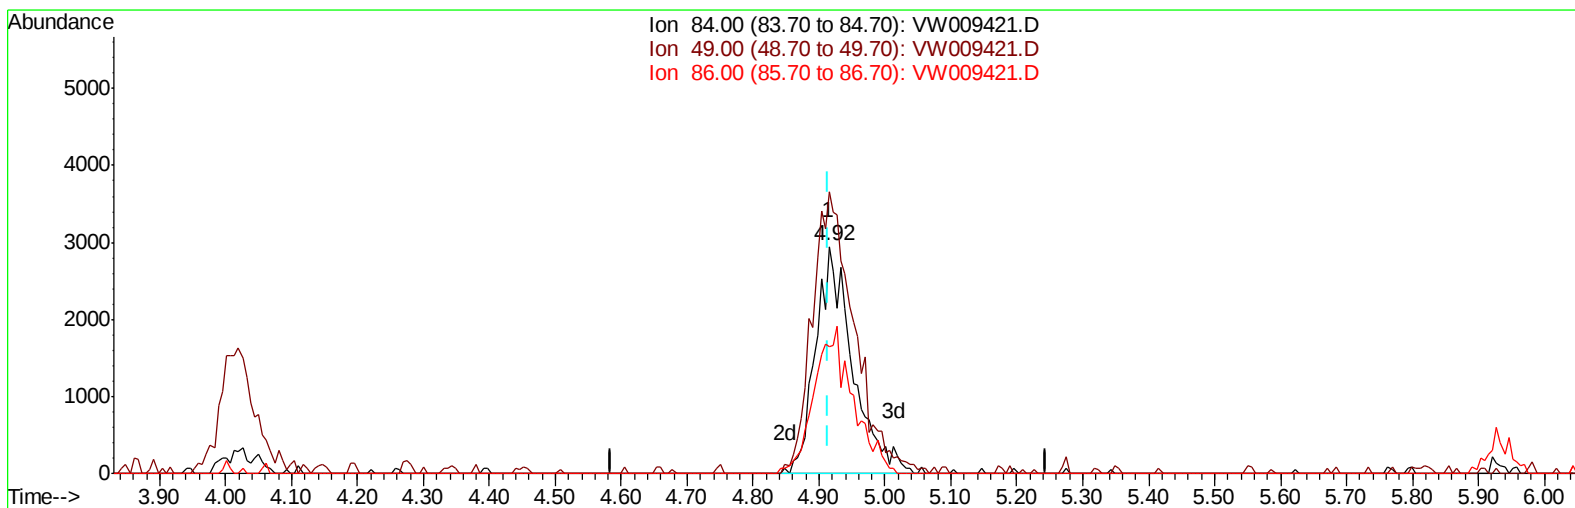

TIC: VW009421.D

(16) Methylene chloride (T)

4.915min (+0.000) 2.28ug/L m

response 11503

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	123.96
86.00	63.50	55.98
0.00	0.00	0.00