
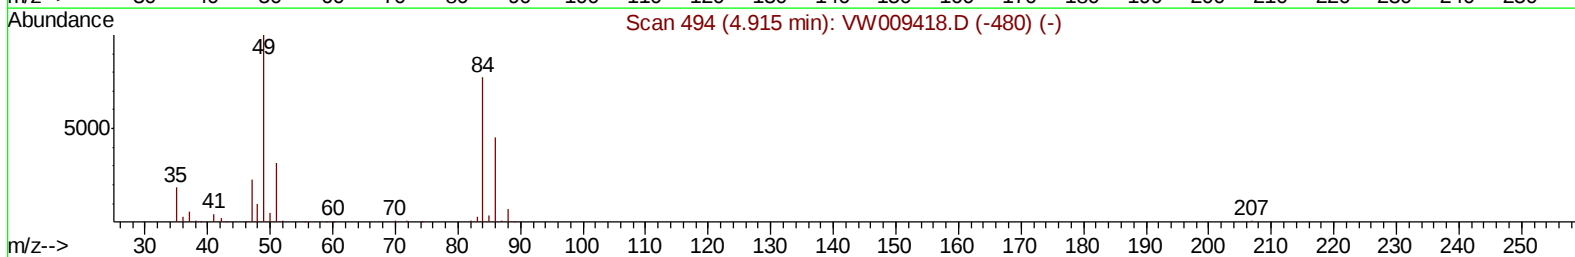
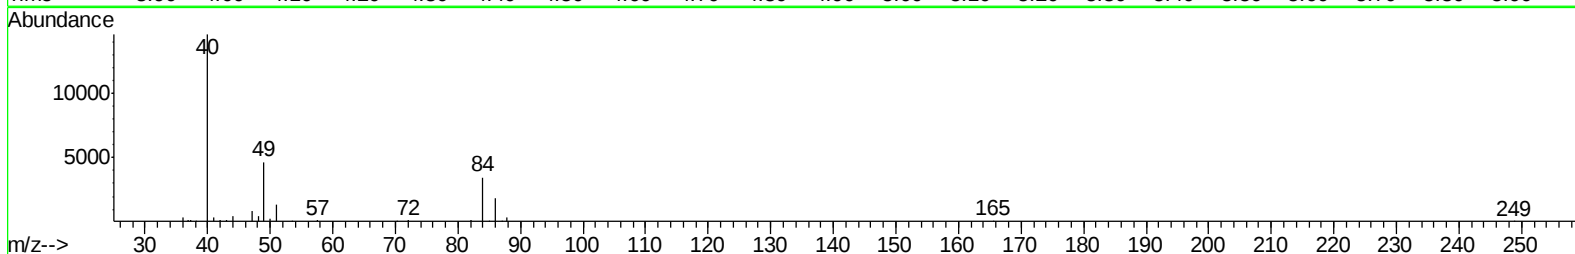


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\  
Data File : VW009426.D  
Acq On : 25 Mar 2019 14:19  
Operator : SY/VA  
Sample : VIBLK15  
Misc : 5.00G/10ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:51:26 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_W\METHOD\SOM2WLM031419S.M  
Quant Title : VOC Analysis  
QLast Update : Tue Mar 26 07:46:05 2019  
Response via : Initial Calibration

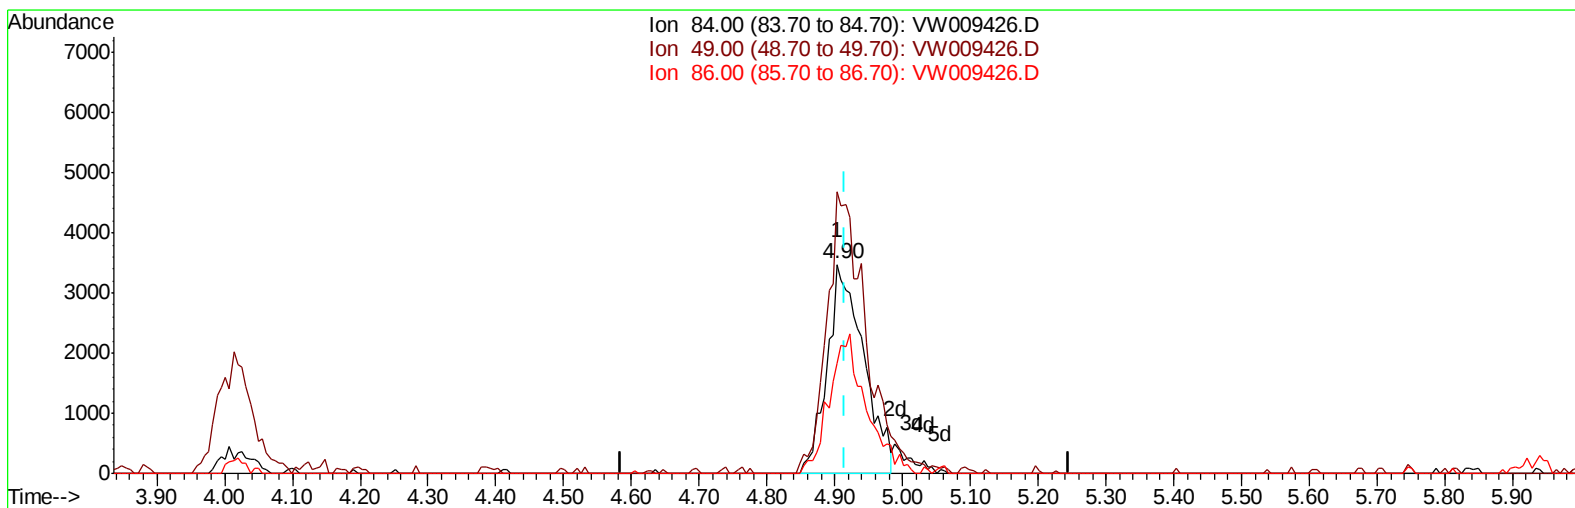

TIC: VW009426.D

(16) Methylene chloride (T)

4.903min (-0.012) 1.94ug/L

response 12894

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 84.00 | 100    | 100    |
| 49.00 | 137.10 | 134.88 |
| 86.00 | 63.50  | 53.00  |
| 0.00  | 0.00   | 0.00   |